

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PANASONIC ; Model No.: MPR-1014R-PT ; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No. : 2K190616069 ; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Dec 2020 ~ 29, Jan 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.2	5.2	3.82	0.18	3.83

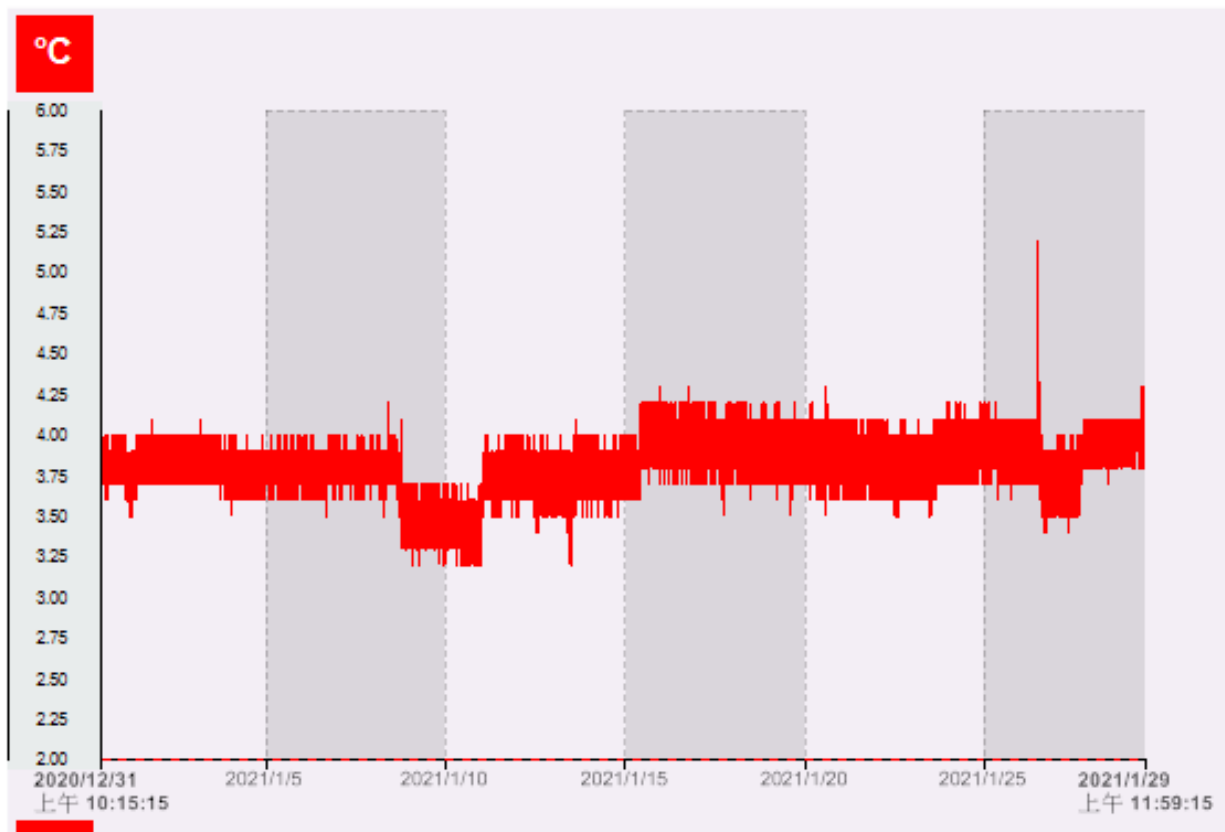

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PANASONIC ; Model No.: MPR-1014R-PT ; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO ; Model No.: KTT 220-O ; Serial No. : 2K190616069 ; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Jan 2021 ~ 26, Feb 2021



KIMO 2K190616069

— v1 [°C]
Min Max Avg Sd MKT
3.3 5.6 3.93 0.19 3.93

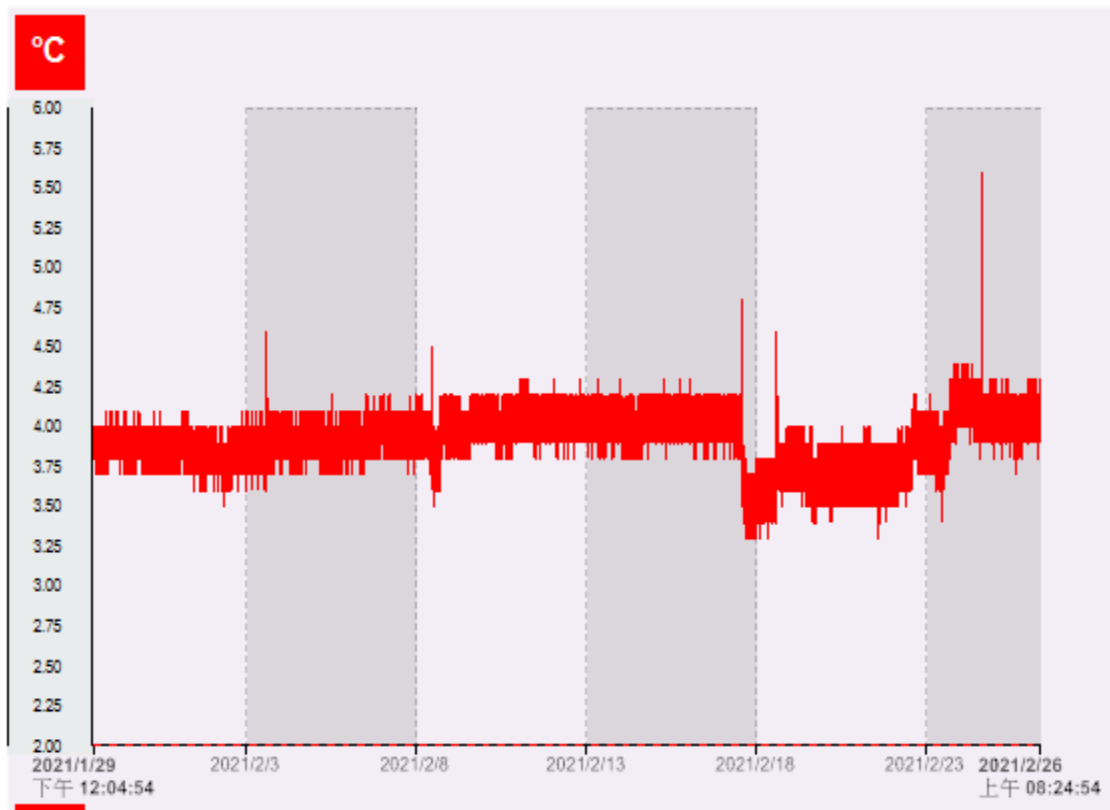

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PANASONIC ; Model No.: MPR-1014R-PT ; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO ; Model No.: KTT 220-O ; Serial No. : 2K190616069 ; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 26, Feb 2021 ~ 31, Mar 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.5	5.1	4.20	0.23	4.21

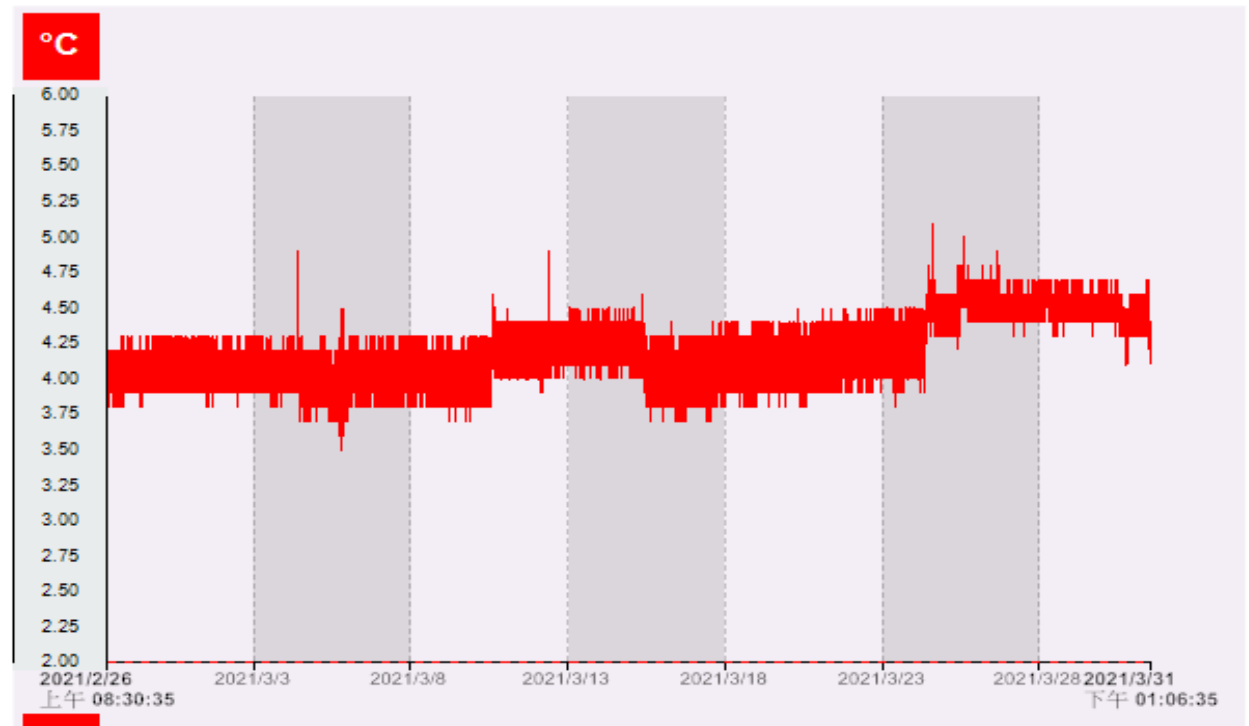

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PANASONIC ; Model No.: MPR-1014R-PT ; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO ; Model No.: KT220-O ; Serial No. : 2K190616069 ; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Mar 2021 ~ 29, Apr 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	5.1	3.90	0.21	3.90

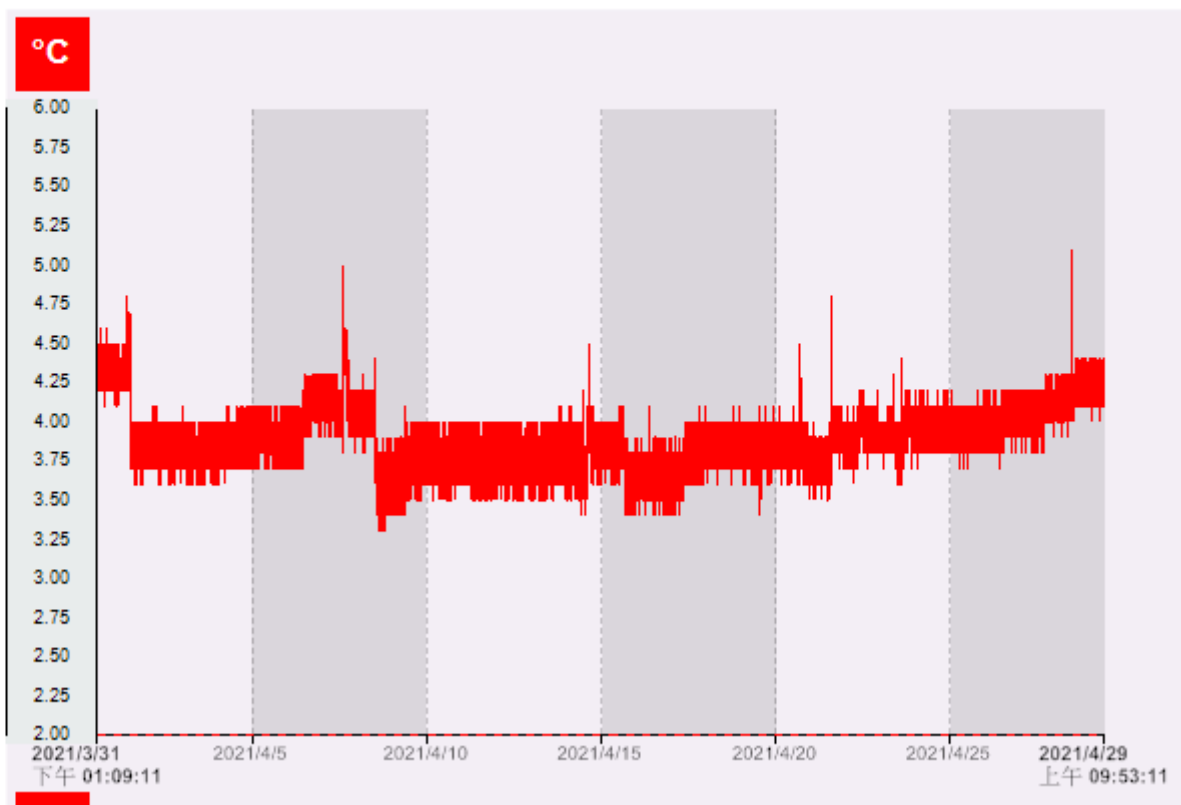

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Apr 2021 ~ 31, May 2021



KIMO 2K190616069

— v1 [°C]				
Min	Max	Avg	Sd	MKT
3.4	5.0	4.00	0.20	4.00

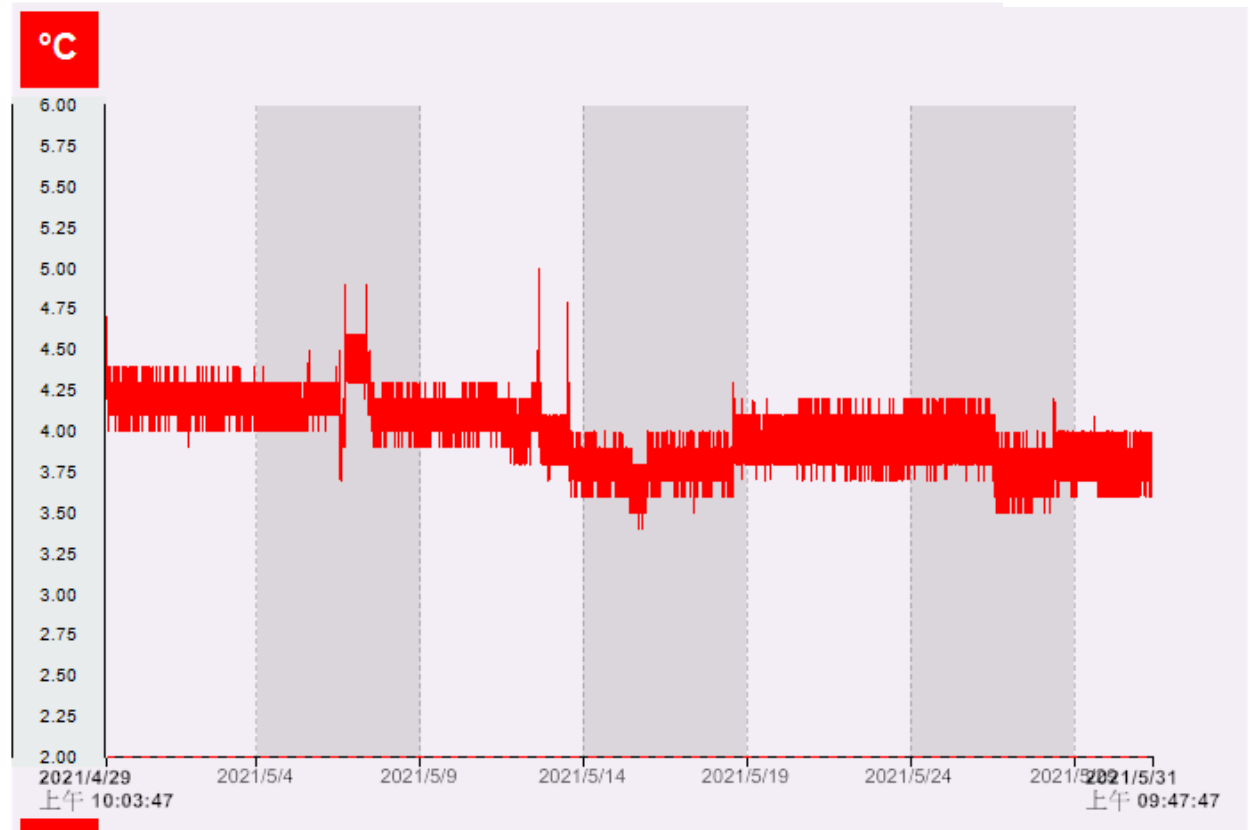

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, May 2021 ~ 30, Jun 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	4.5	3.79	0.16	3.79

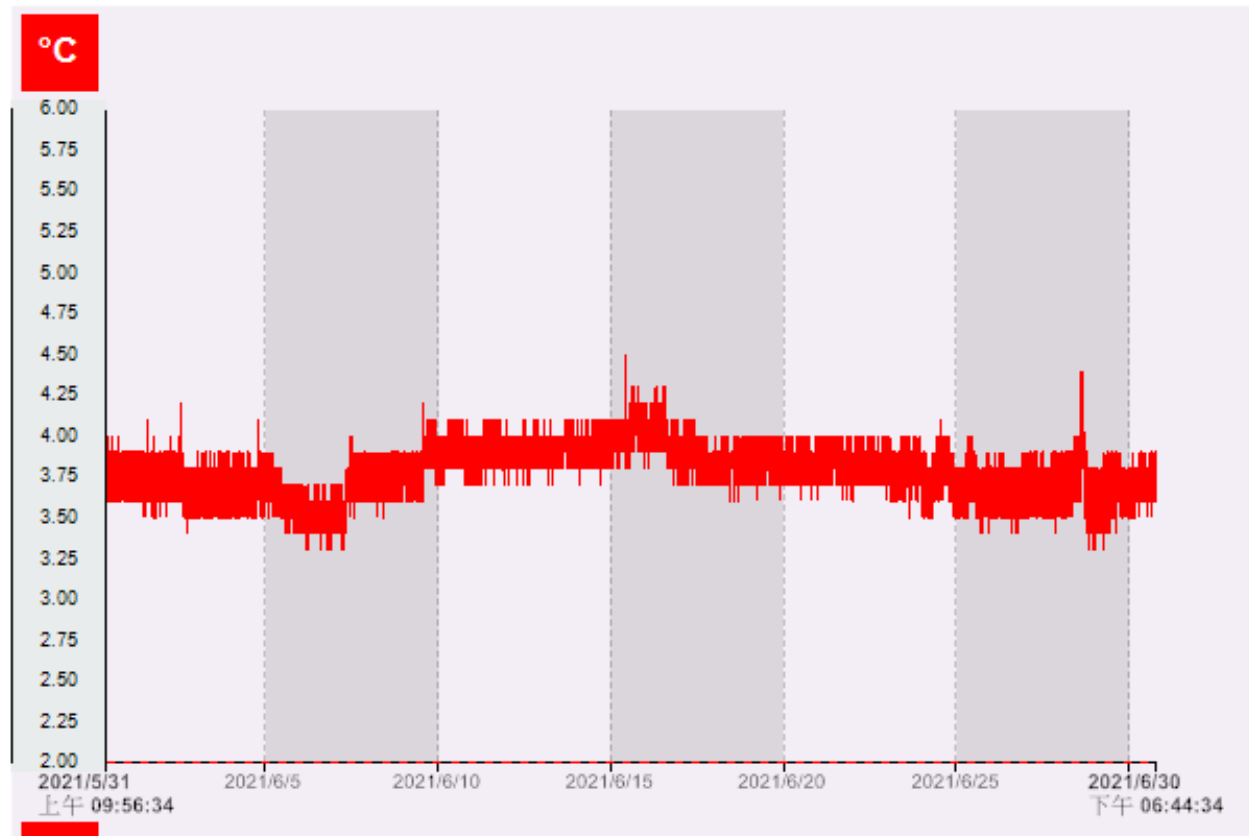

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KT220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Jun 2021 ~ 30, Jul 2021



KIMO 2K160903197

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.4	4.5	3.97	0.19	3.97

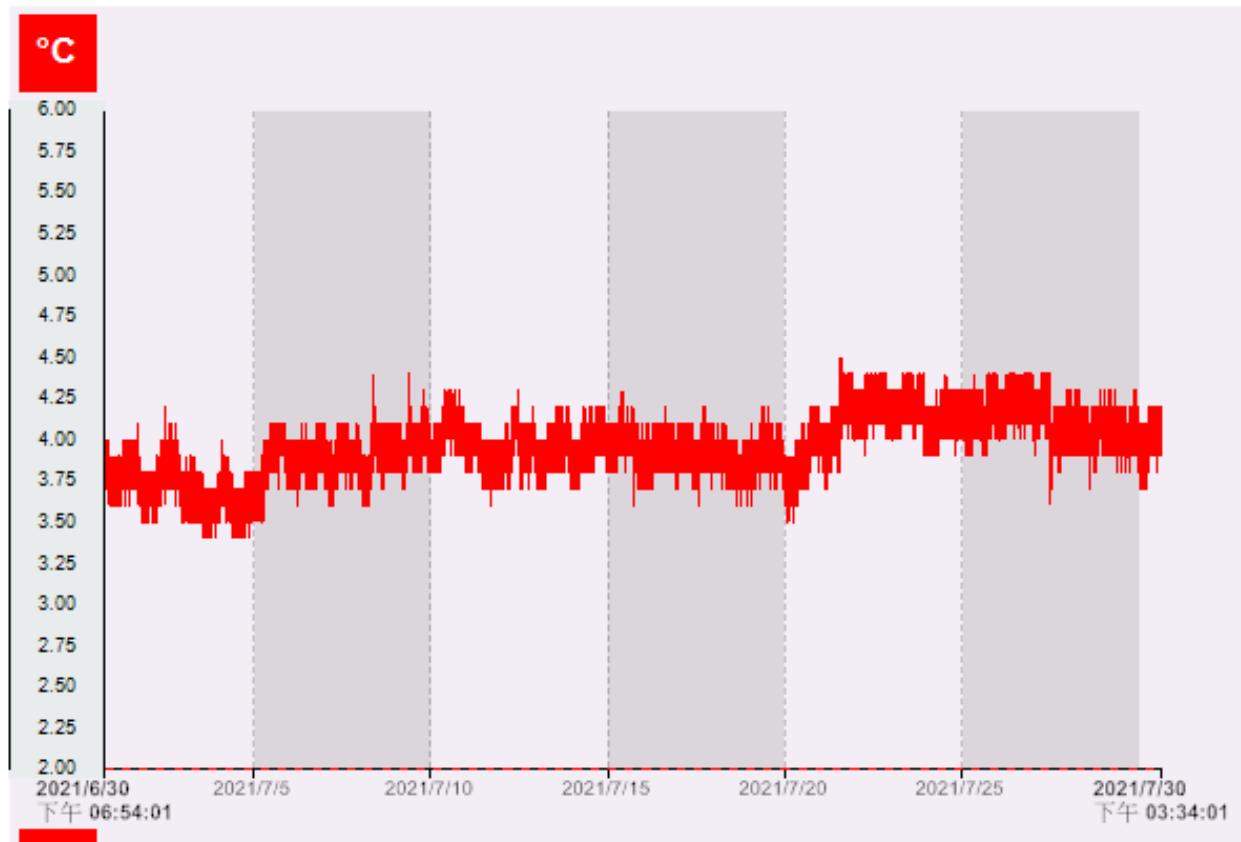

Comment :

本溫度記錄器(2K190616069)於2021年6月30日送校，期間以備品溫度記錄器(2K160903197)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KT220-O; Serial No.: 2K190616069; Channel No.: 1

REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Jul 2021 ~ 31, Aug 2021



KIMO 2K160903197

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	6.7	3.94	0.20	3.94



Comment :

本溫度記錄器(2K190616069)於2021年6月30日送校，期間以備品溫度記錄器(2K160903197)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Aug 2021 ~ 30, Sep 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.9	4.8	3.79	0.30	3.80

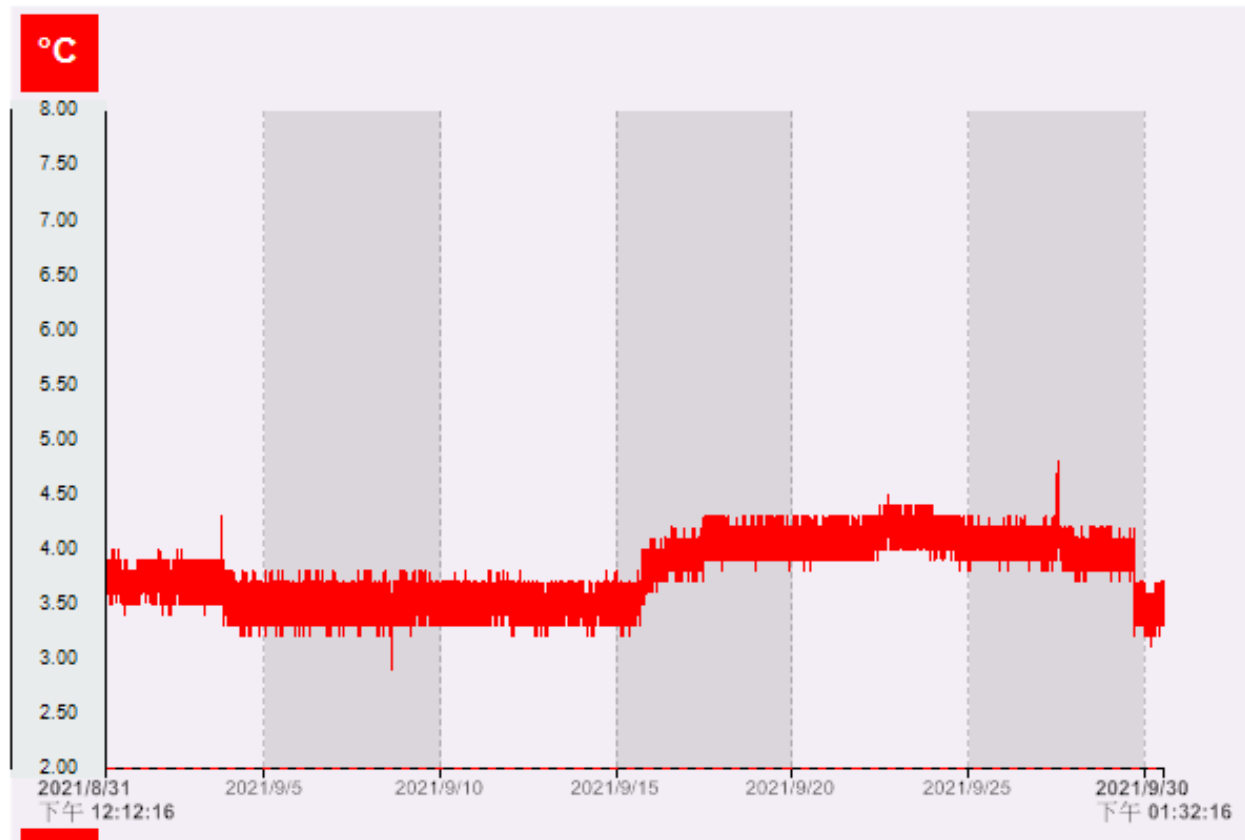

Comment : 因下載溫度用之筆電的時間有誤差，此月份溫度記錄之開始與結束時間比實際時間晚3hr 9

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Sep 2021 ~ 29, Oct 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.8	4.4	3.45	0.24	3.45

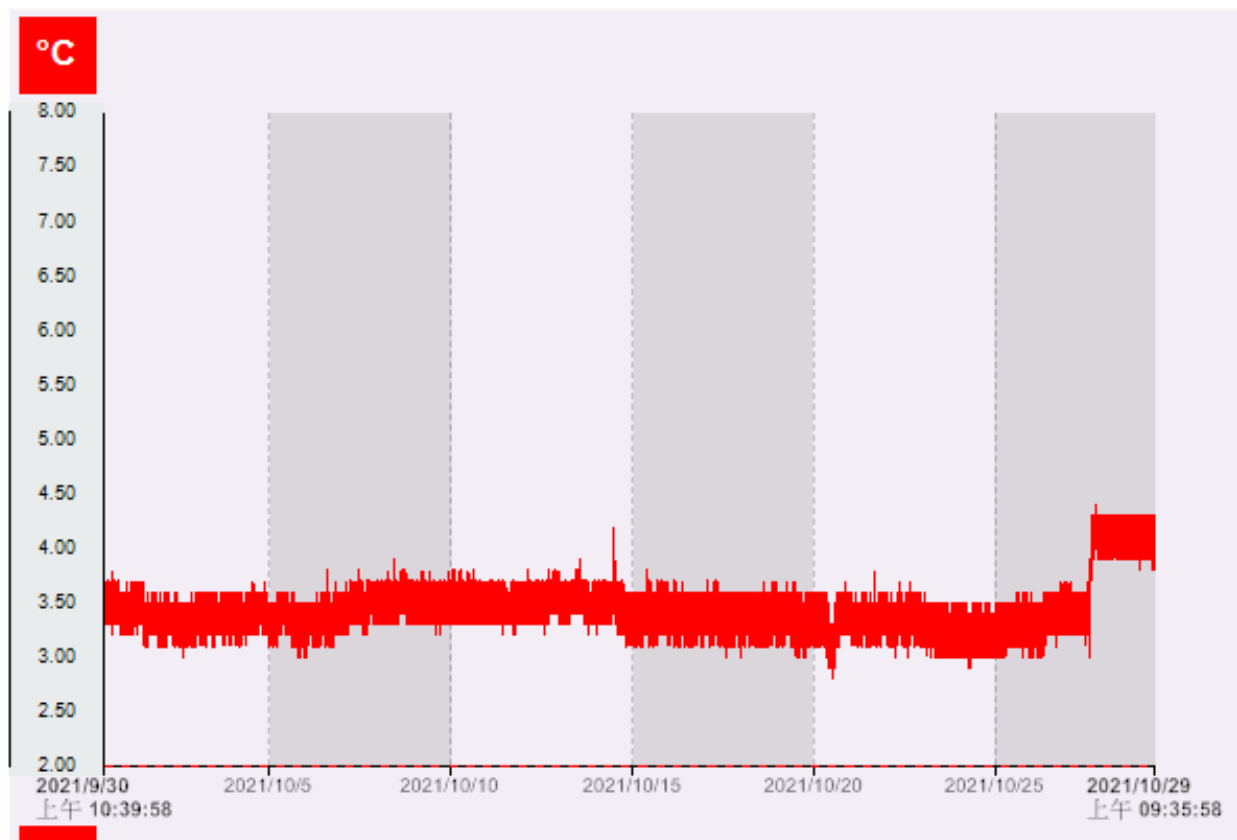

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTТ 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Oct 2021 ~ 30, Nov 2021



KIMO 2K190616069

— v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	5.0	4.03	0.25	4.03

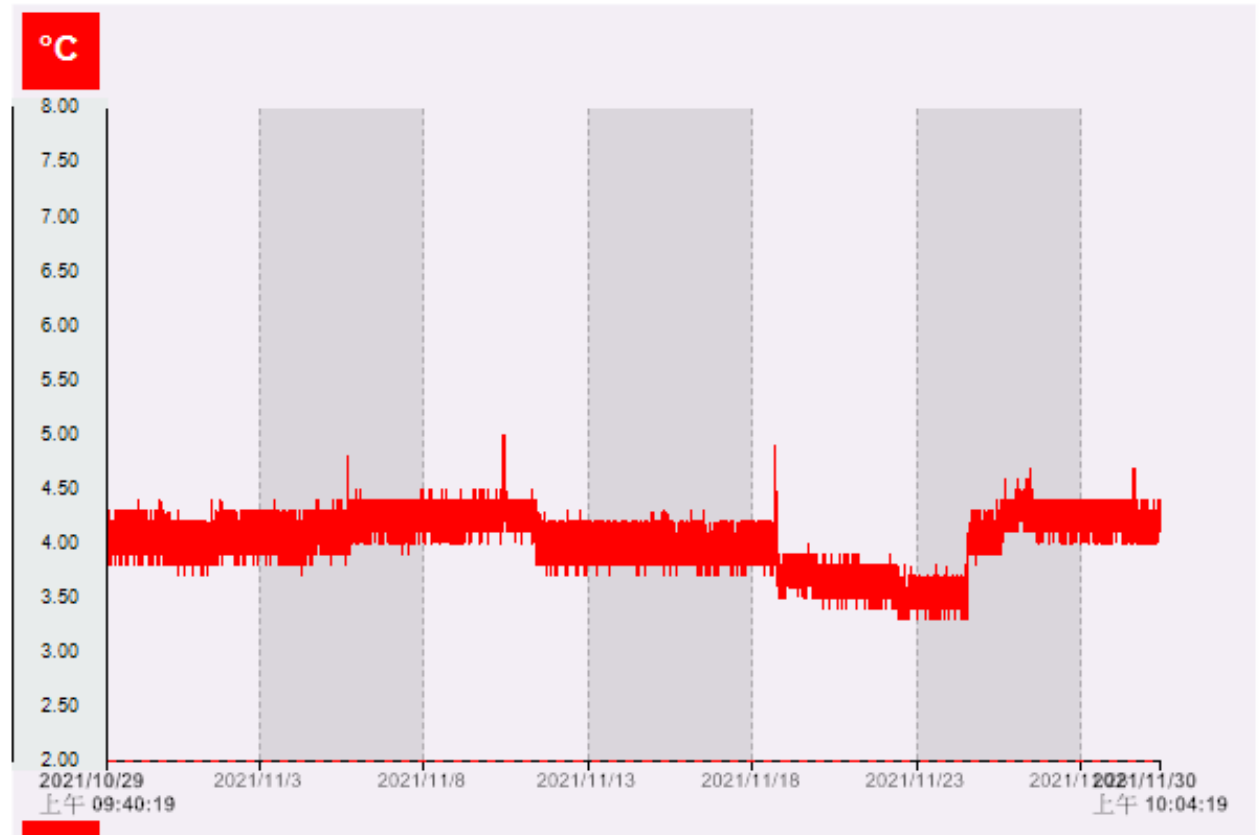

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Nov 2021 ~ 29, Dec 2021



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.9	5.3	3.73	0.38	3.73

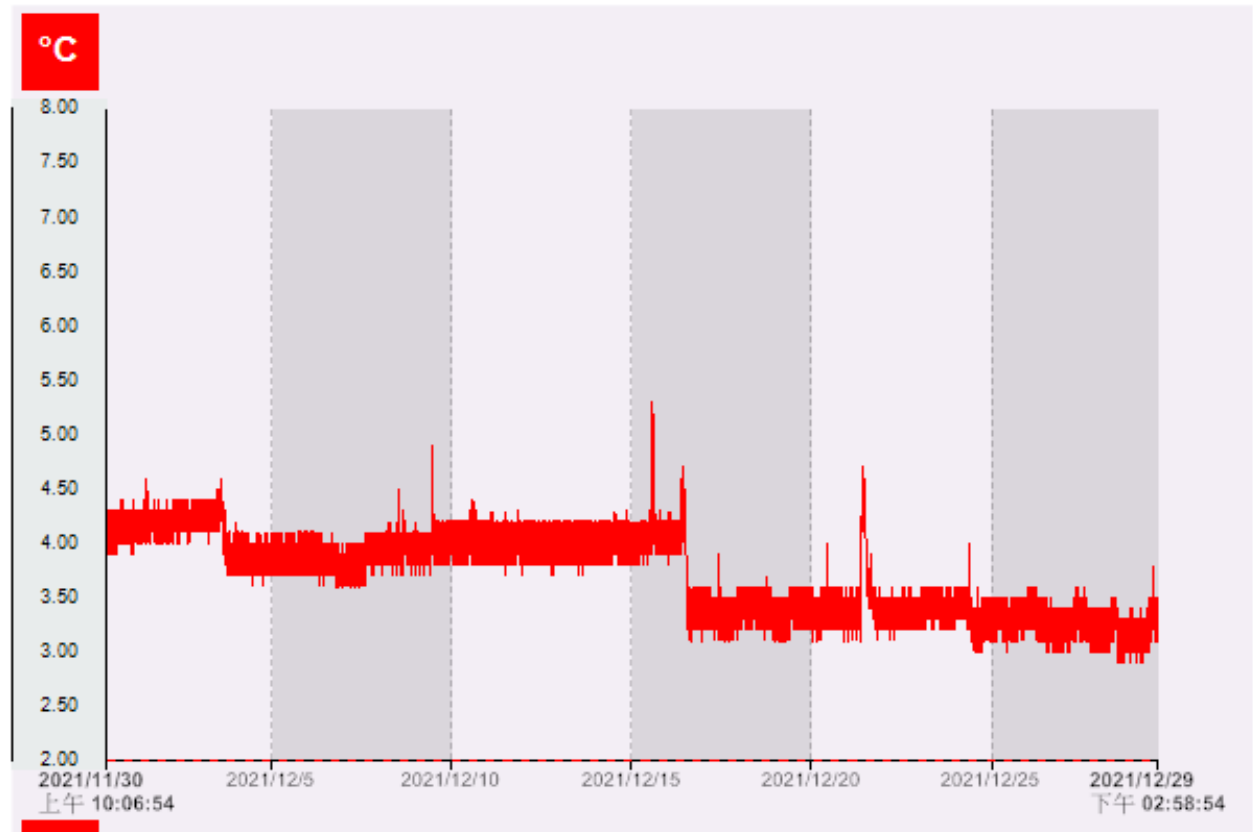

Comment :