

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 01, Jun 2022 ~ 28, Jun 2022

Instrument name: Testo 176T2		2022/6/28 04:39:12			Page	1/1
Start time: 2022/6/1 10:09:01		Minimum	Maximum	Mean value	Limit values	
End time: 2022/6/28 10:09:01	40505446 [°C]	-70.74	-67.70	-68.682	-80.0/-60.0	
Measurement channels: 1						
Measured values: 649						
SN 40505446						

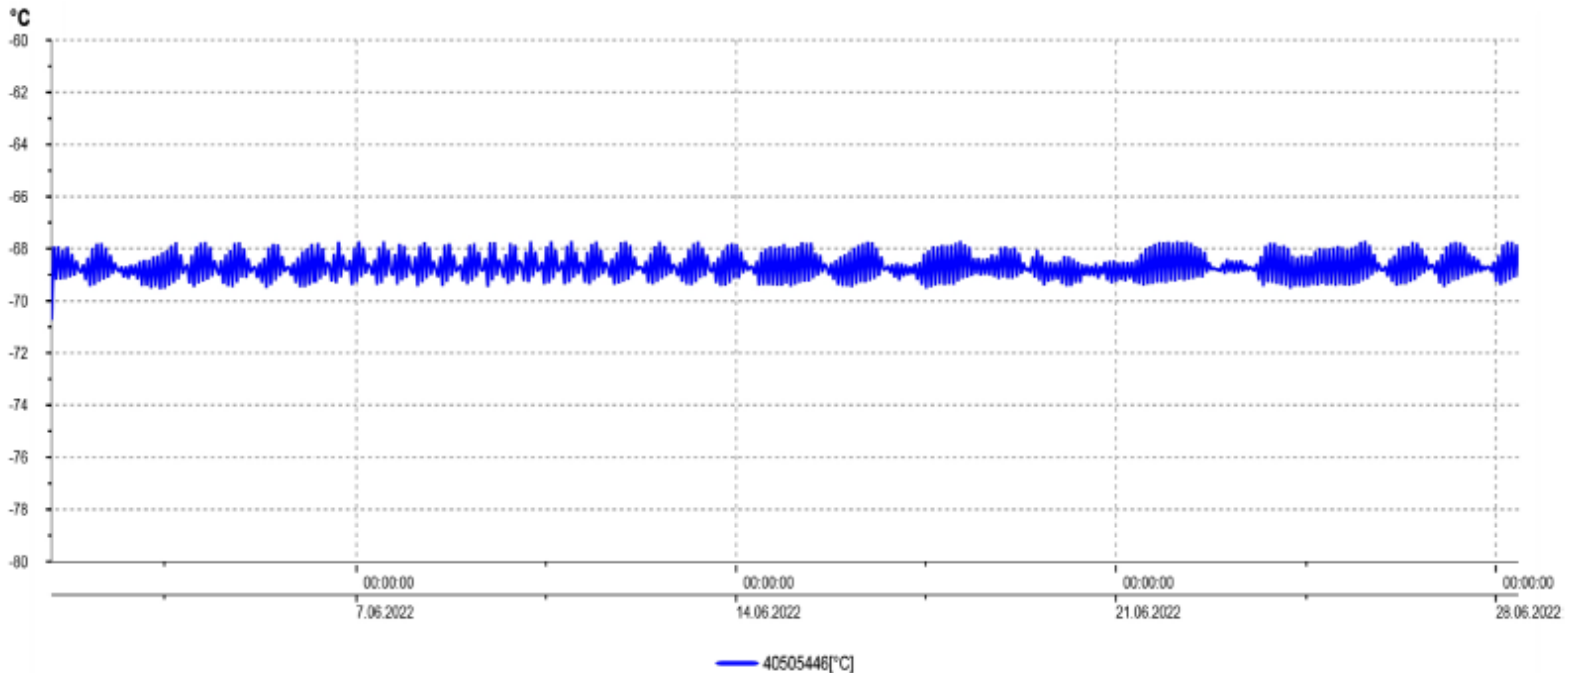

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-310 ; Serial No. : 1201 0863; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 21, Jul 2022 ~ 29, Jul 2022

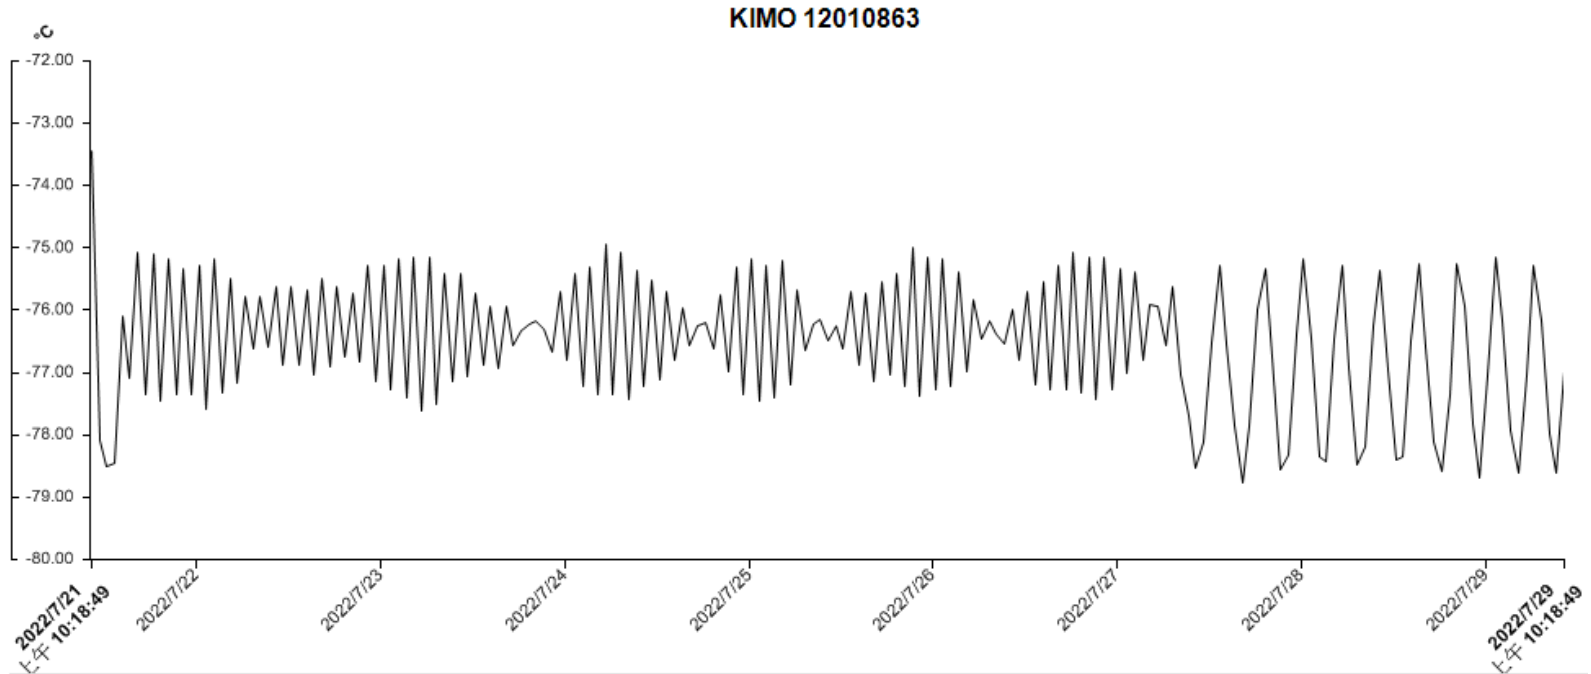

統計表

#1	
最小 T	-78.78
最小 t	-78.78
最大值 T	-73.44
最大值 t	-73.44
平均值 T	-76.511
平均值 t	-76.511
標準偏差 T	1.037
標準偏差 t	1.037
MKT T	-76.516
MKT t	-76.516

T: 整個週期
t: 顯示週期

Comment: 溫度記錄器於2022年7月21日10:18更換為1201 0863，並暫時存放-80°C冷凍櫃藥品，待溫度穩定後於2022年7月21日14:41將藥品移回-80°C冷凍櫃。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 29, Jul 2022 ~ 31, Aug 2022

Instrument name: Testo 176T2		2022/9/1 ☐☐ 11:13:16			Page	1/1
Start time: 2022/7/29 ☐☐ 01:07:00		Minimum	Maximum	Mean value	Limit values	
End time: 2022/8/31 ☐☐ 04:07:00	40505446 [°C]	-77.41	-62.38	-72.286	-80.0/-60.0	
Measurement channels: 1						
Measured values: 796						
SN 40505446						

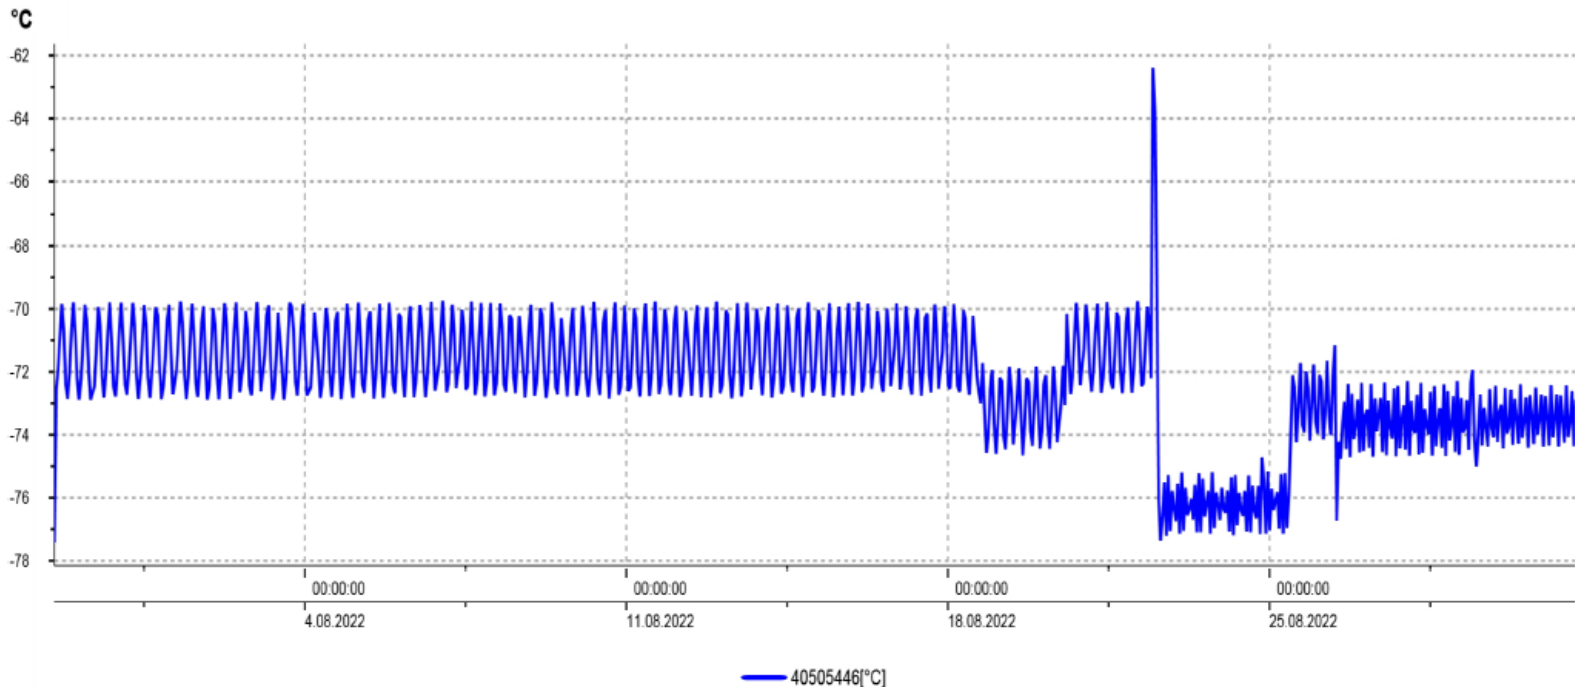

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31, Aug 2022 ~ 30, Sep 2022

Instrument name: Testo 176T2		2022/9/30 下午 04:30:34			Page 1/1
Start time: 2022/8/31 下午 04:33:29		Minimum	Maximum	Mean value	Limit values
End time: 2022/9/30 下午 02:33:29	40505446 [°C]	-76.05	-69.27	-73.139	-80.0/-60.0
Measurement channels: 1					
Measured values: 719					
SN 40505446					

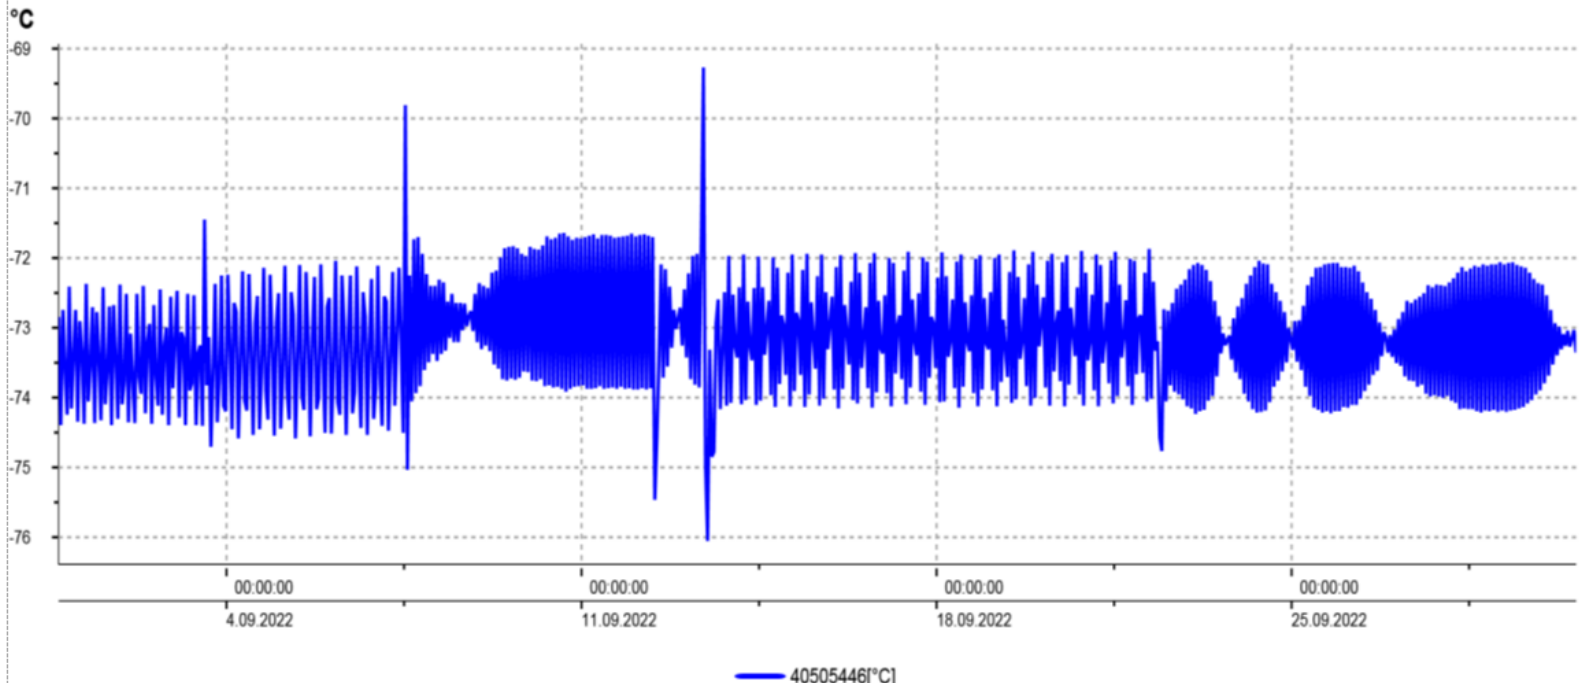

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 30, Sep 2022 ~ 28, Oct 2022

Instrument name: Testo 176T2		2022/10/28 下午 02:43:07			Page 1/1
Start time: 2022/9/30 下午 03:15:48		Minimum	Maximum	Mean value	Limit values
End time: 2022/10/28 下午 02:15:48	40505446 [°C]	-74.29	-71.95	-73.170	-80.0/-60.0
Measurement channels: 1					
Measured values: 672					
SN 40505446					

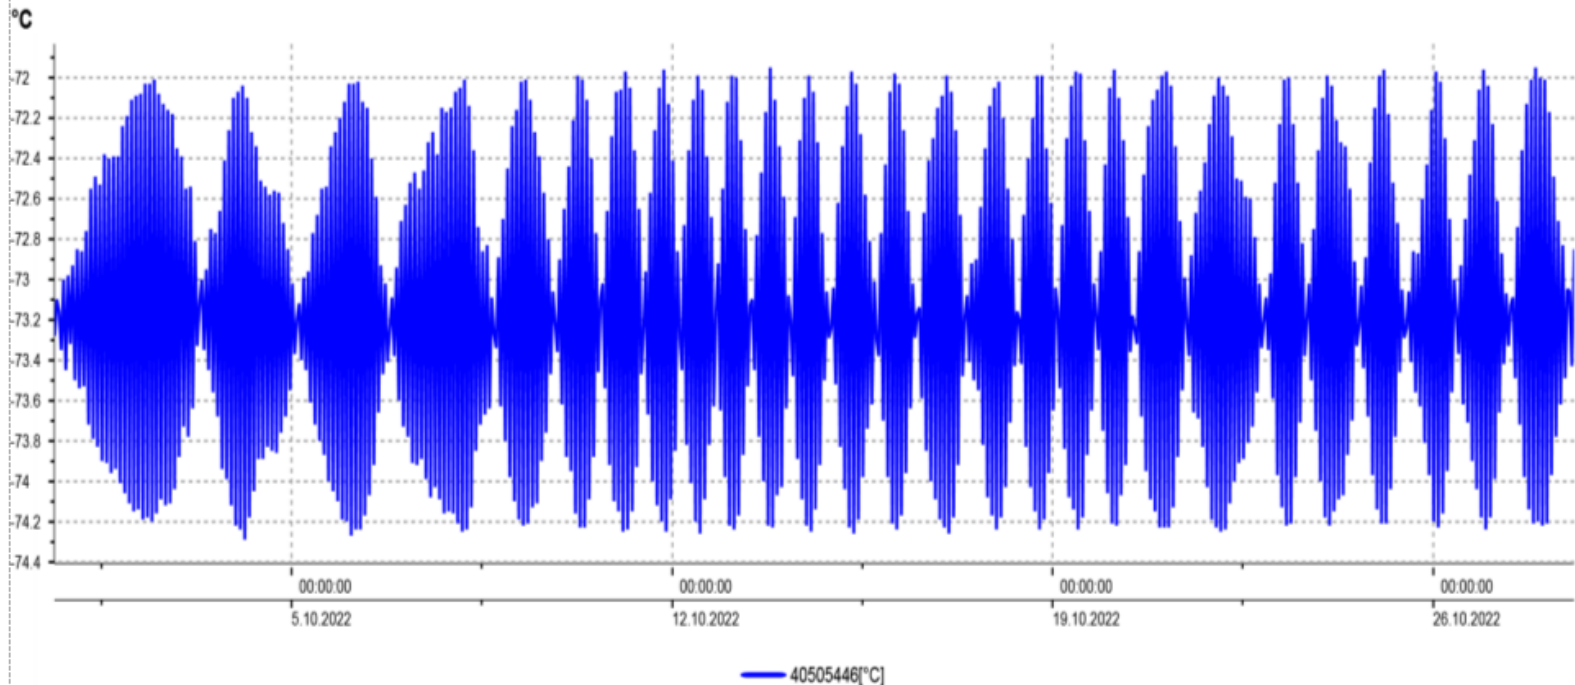

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 28, Oct 2022 ~ 30, Nov 2022

Instrument name: Testo 176T2		2022/11/30 下午 02:46:11			Page 1/1
Start time: 2022/10/28 下午 02:28:21		Minimum	Maximum	Mean value	Limit values
End time: 2022/11/30 下午 02:28:21	40505446 [°C]	-74.19	-71.88	-73.097	-80.0/-60.0
Measurement channels: 1					
Measured values: 793					
SN 40505446					

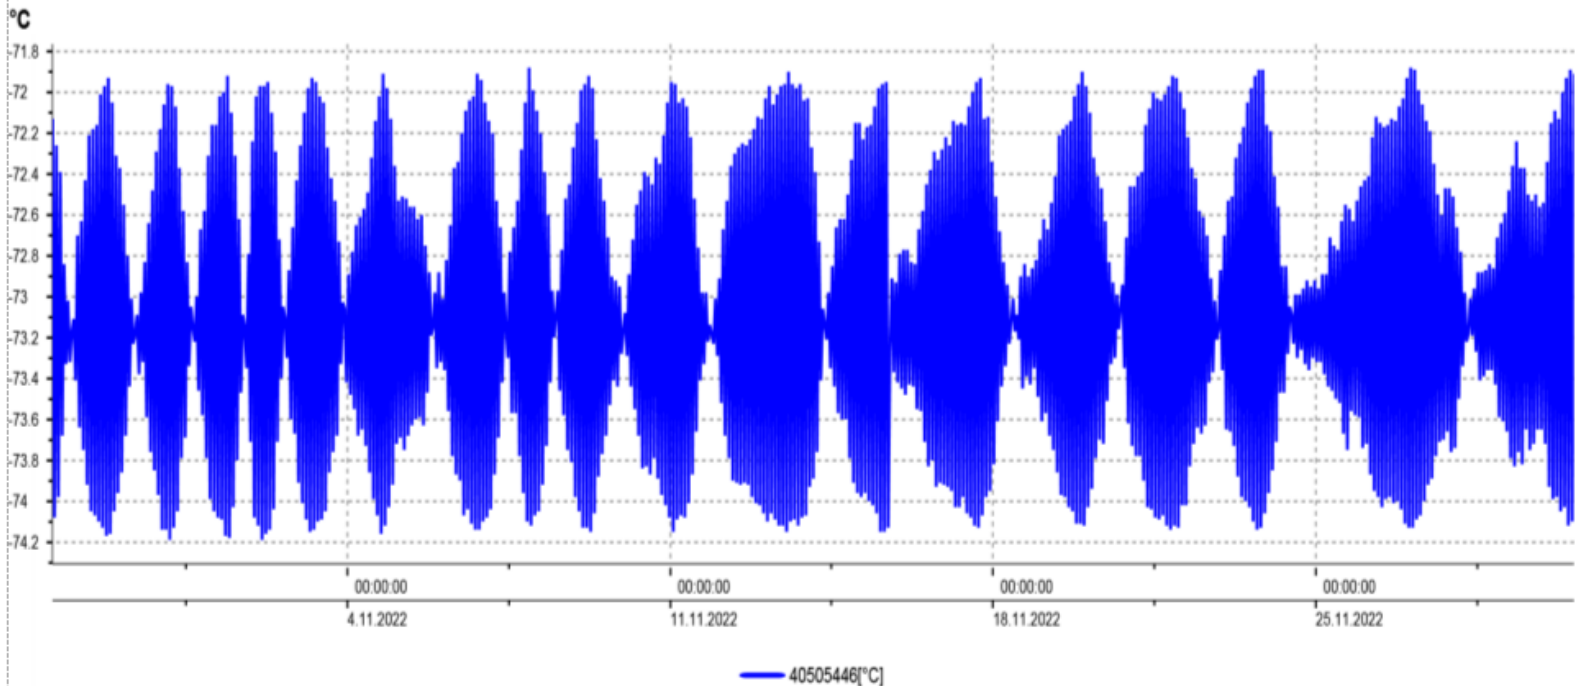

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 30, Nov 2022 ~ 03, Jan 2023

Instrument name: Testo 176T2		2023/1/3 上午 11:38:07			Page 1/1
Start time: 2022/11/30 下午 02:31:48		Minimum	Maximum	Mean value	Limit values
End time: 2023/1/3 上午 10:31:48	40505446 [°C]	-74.15	-71.77	-73.038	-80.0/-60.0
Measurement channels: 1					
Measured values: 813					
SN 40505446					

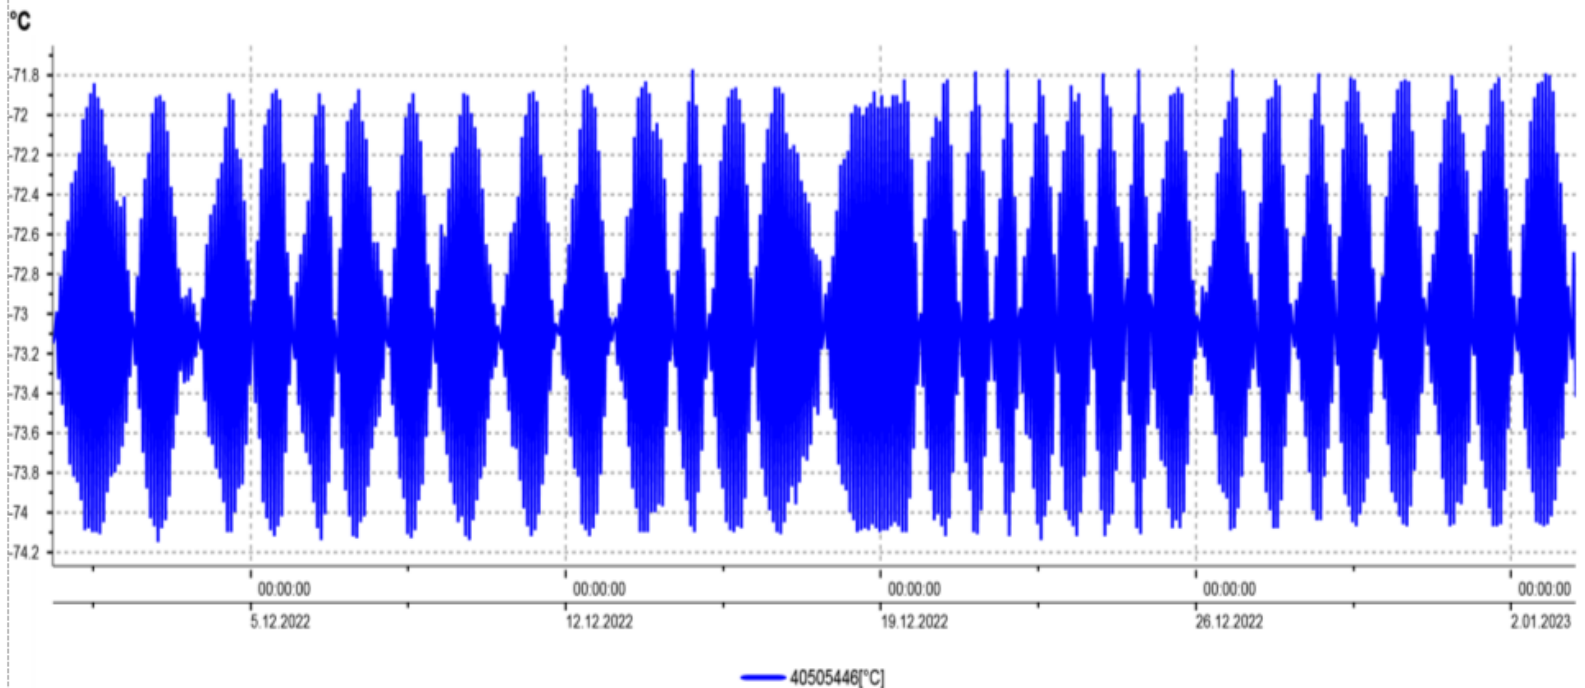

Comment: