

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 29, Dec 2021 ~ 25, Jan 2022



2K190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.0 -72.8 -80.11 0.55 -80.06

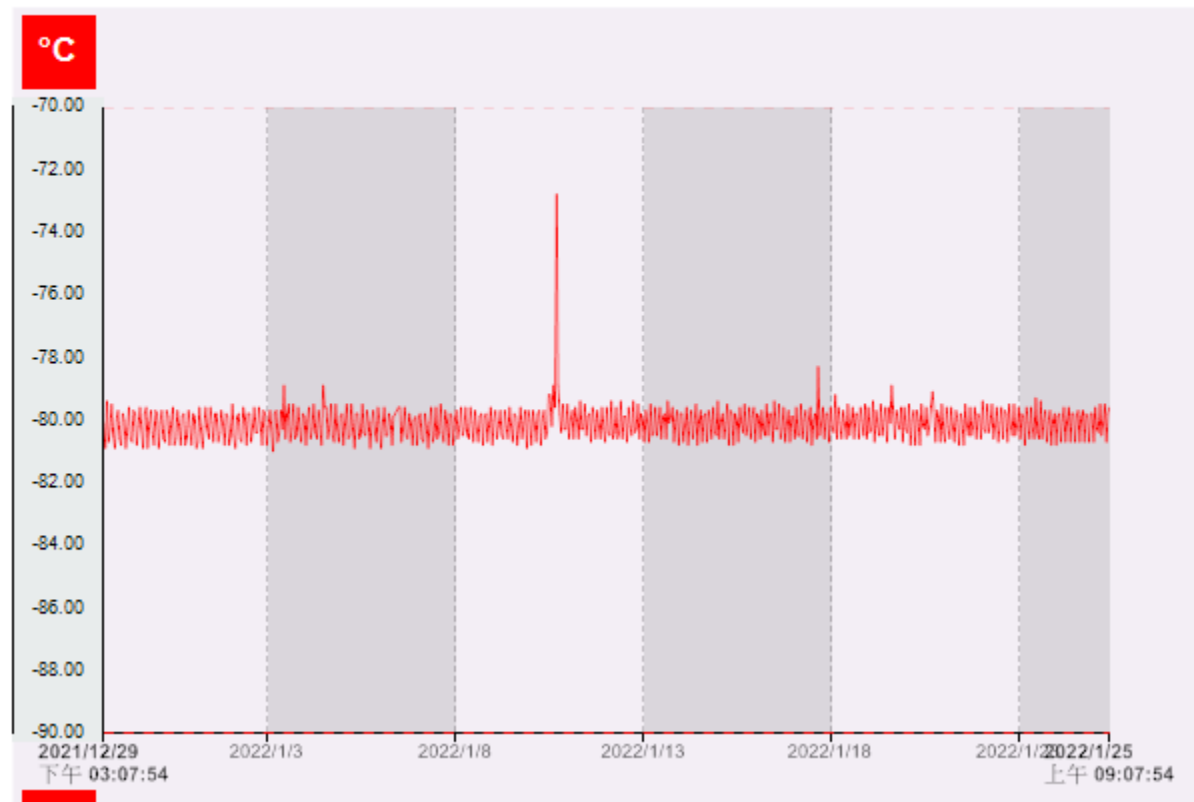

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 25, Jan 2022 ~ 24, Feb 2022



2K190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.0 -74.9 -80.11 0.50 -80.08

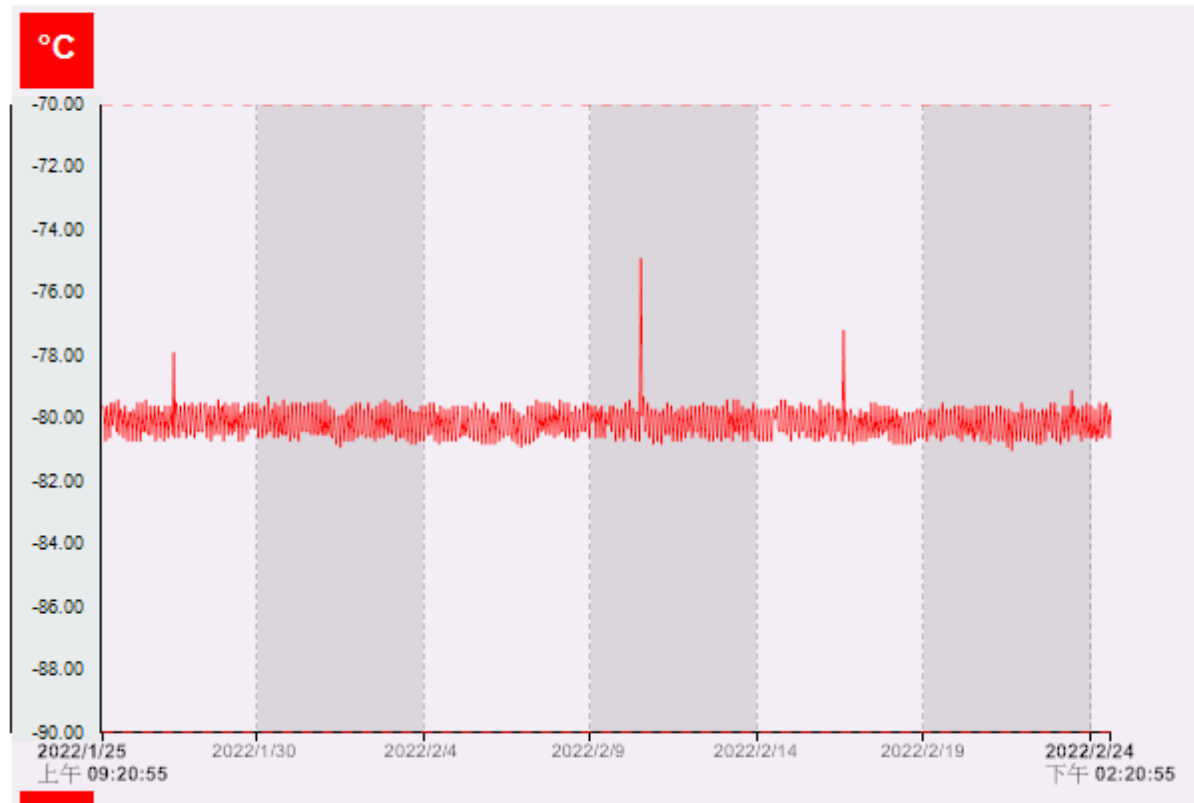

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C


DATE : 24, Feb 2022 ~ 31, Mar 2022



2K190114208

20

— v1 [°C]
Min Max Avg Sd MKT
-80.9 -73.9 -80.09 0.50 -80.06

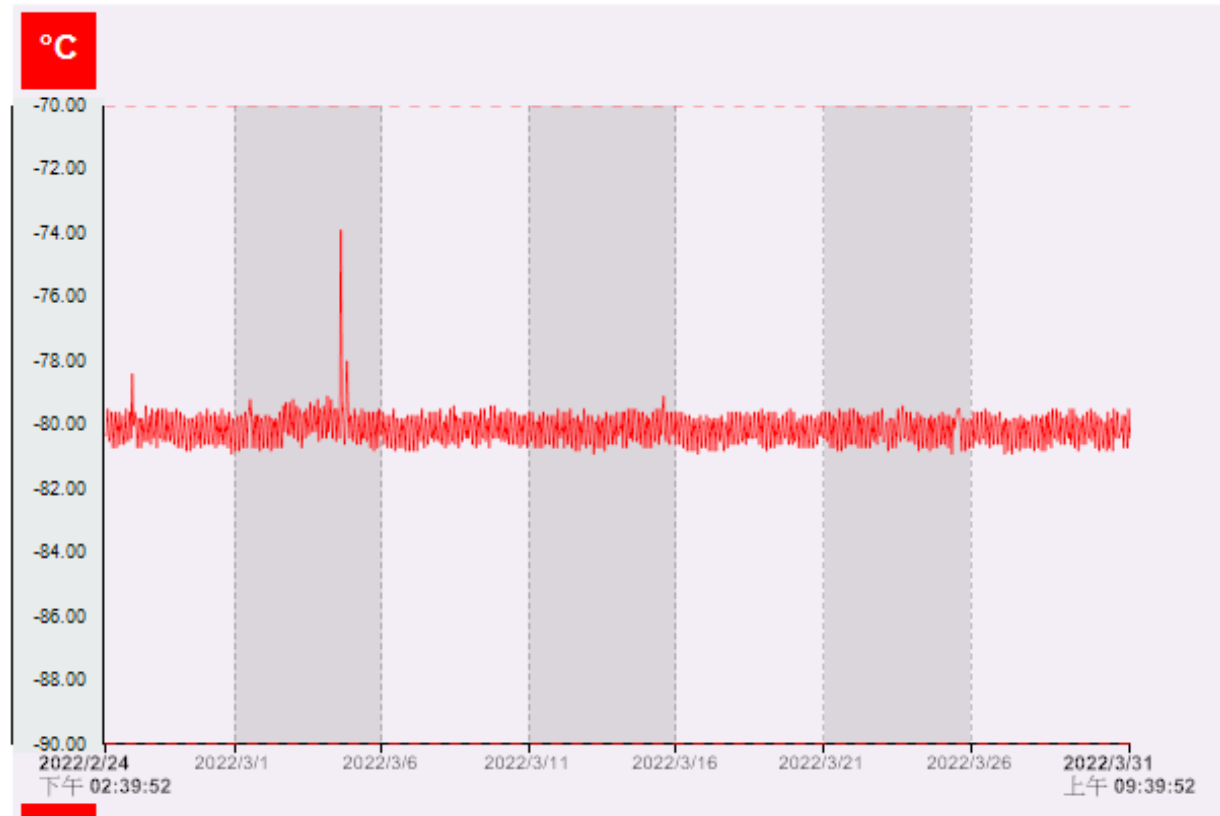

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : $-80 \pm 10 \text{ }^\circ\text{C}$

DATE : 31, Mar 2022 ~ 29, Apr 2022



2K190114208

— v1 [°C]
Min Max Avg Sd MKT
-80.9 -74.5 -80.08 0.48 -80.04

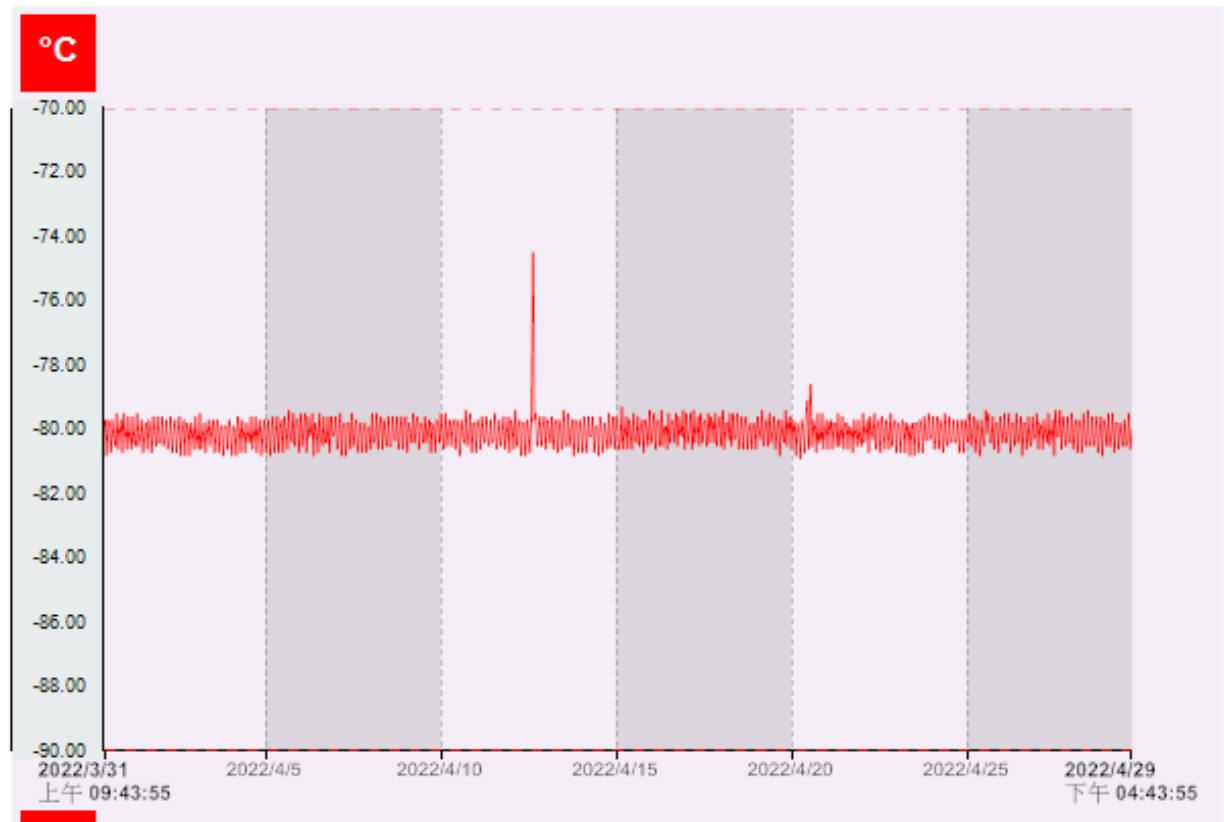

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 29, Apr 2022 ~ 30, May 2022



2K190114208

v1 [°C]
Min Max Avg Sd MKT
-80.9 -76.2 -80.02 0.47 -79.99

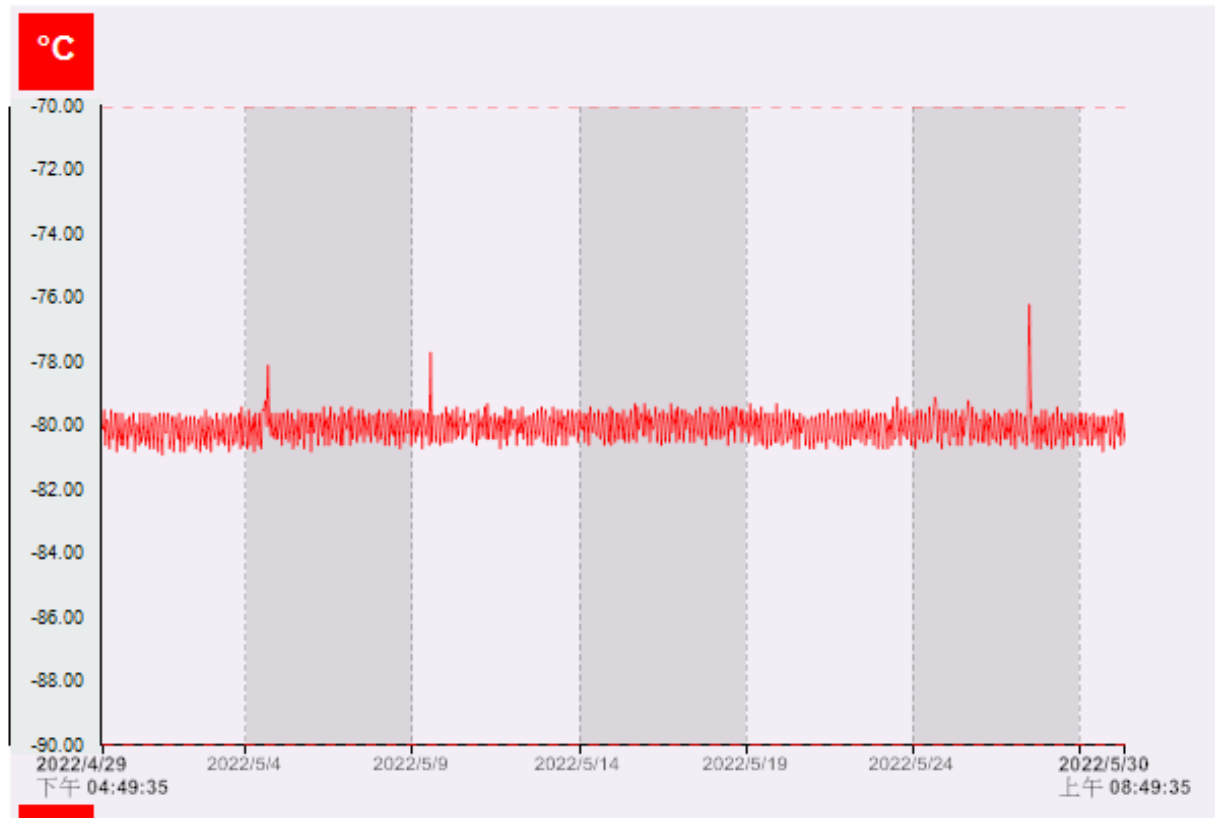

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT220-0 ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 30, May 2022 ~ 28, Jun 2022



2K190114208

v1 [°C]
Min Max Avg Sd MKT
-80.9 -77.6 -80.08 0.45 -80.05

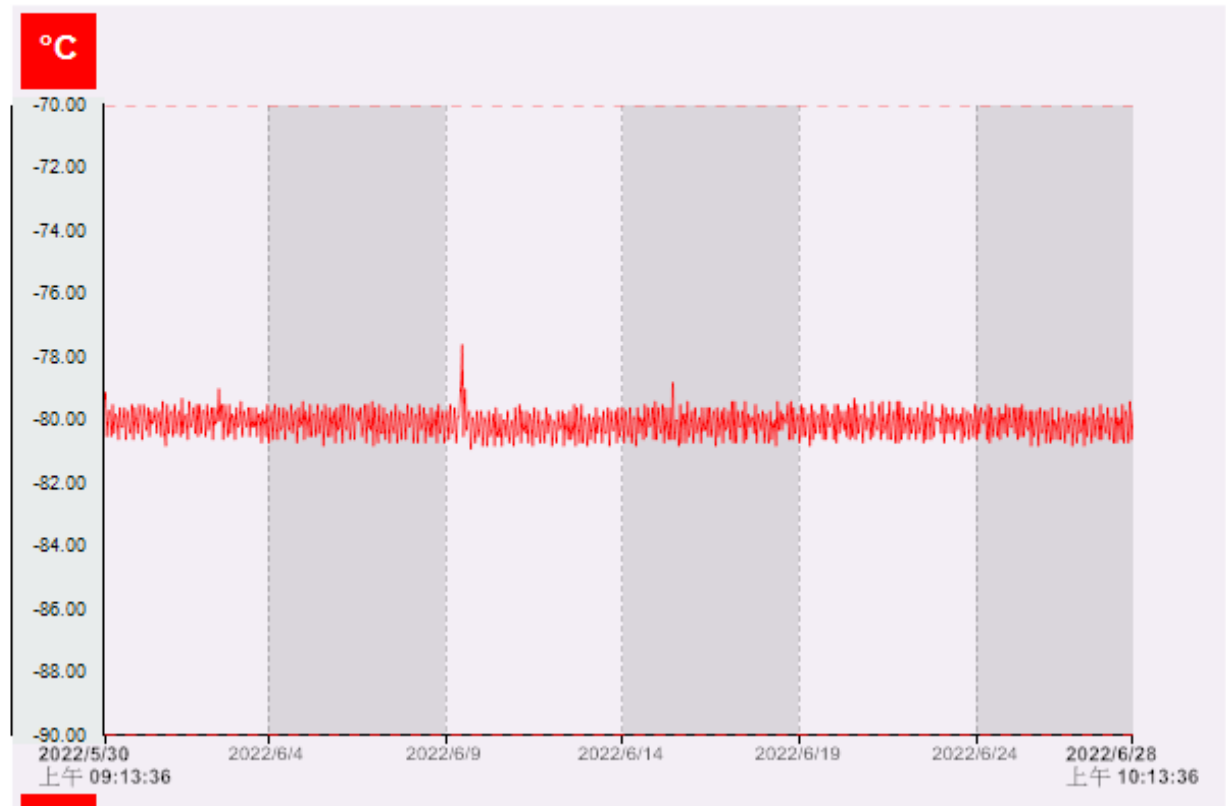

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-310 ; Serial No. : 1201 0863; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 28, Jun 2022 ~ 21, Jul 2022

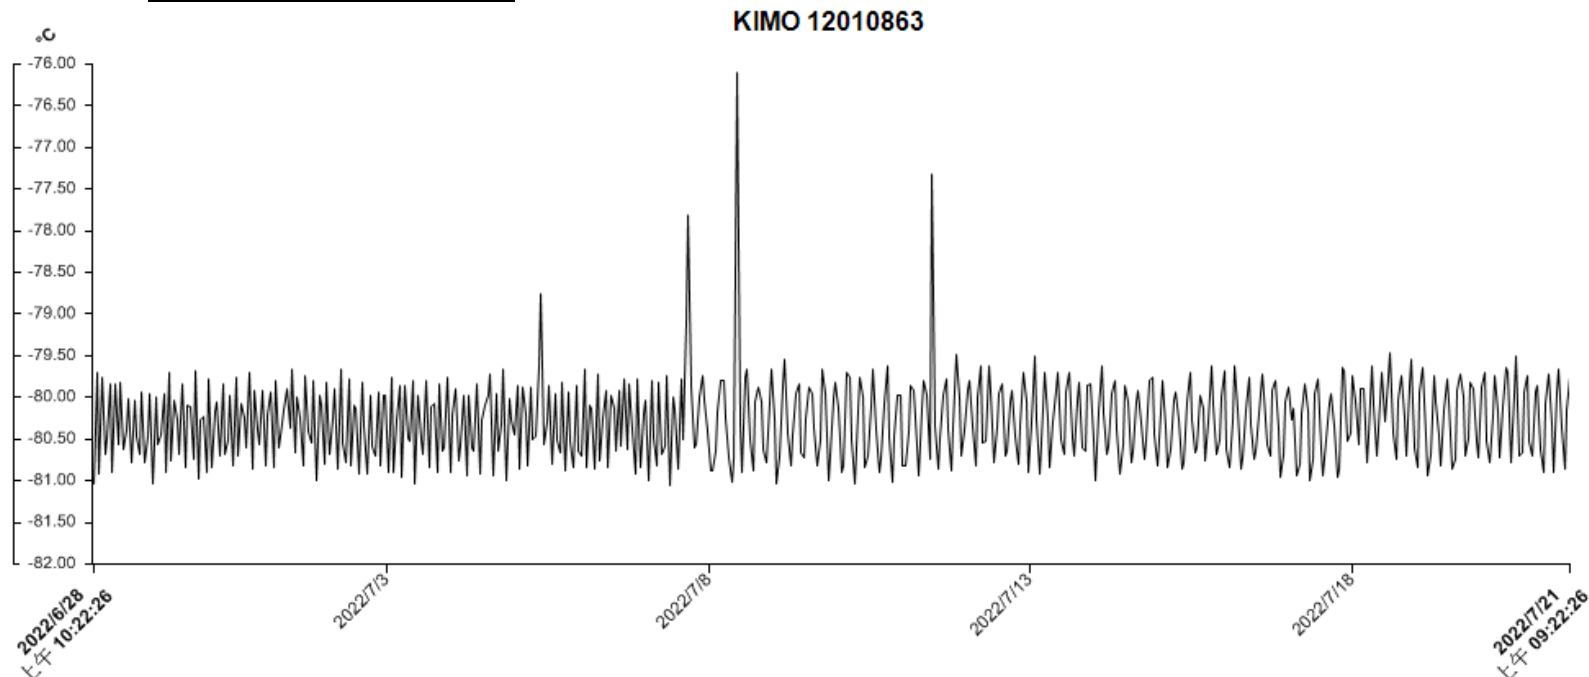

統計表

#1	
最小 T	-81.06
最小 t	-81.06
最大值 T	-76.09
最大值 t	-76.09
平均值 T	-80.272
平均值 t	-80.272
標準偏差 T	0.494
標準偏差 t	0.494
MKT T	-80.273
MKT t	-80.273

T: 整個週期
t: 顯示週期

Comment: 本溫度記錄器(2K190114208)於2022年6月28日送校，期間以備品溫度記錄器(1201 0863)暫代。於2022年7月21日更換溫度記錄器的感溫線，調整感溫探頭，並於10:18藥品暫時移至-70°C冷凍櫃。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 21, Jul 2022 ~ 29, Jul 2022



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.3 -73.7 -79.88 1.04 -79.72

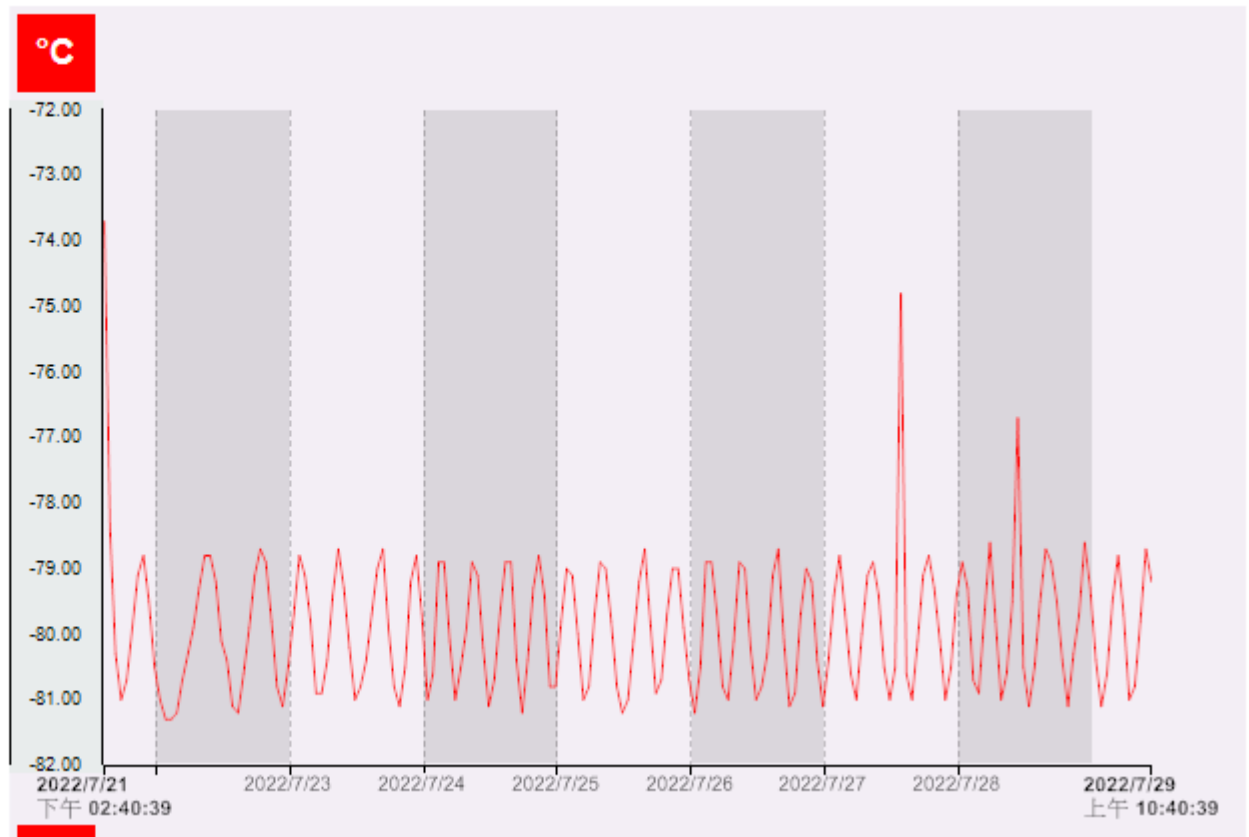

Comment: 於2022年7月21日除霜之後，14:41重啟並將藥品移回。本溫度記錄器(2K190114208)於2022年7月11日 8 完成校正。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 29, Jul 2022 ~ 22, Aug 2022



2K 190114208

v1 [°C]				
Min	Max	Avg	Sd	MKT
-81.5	-66.6	-79.89	1.01	-79.66

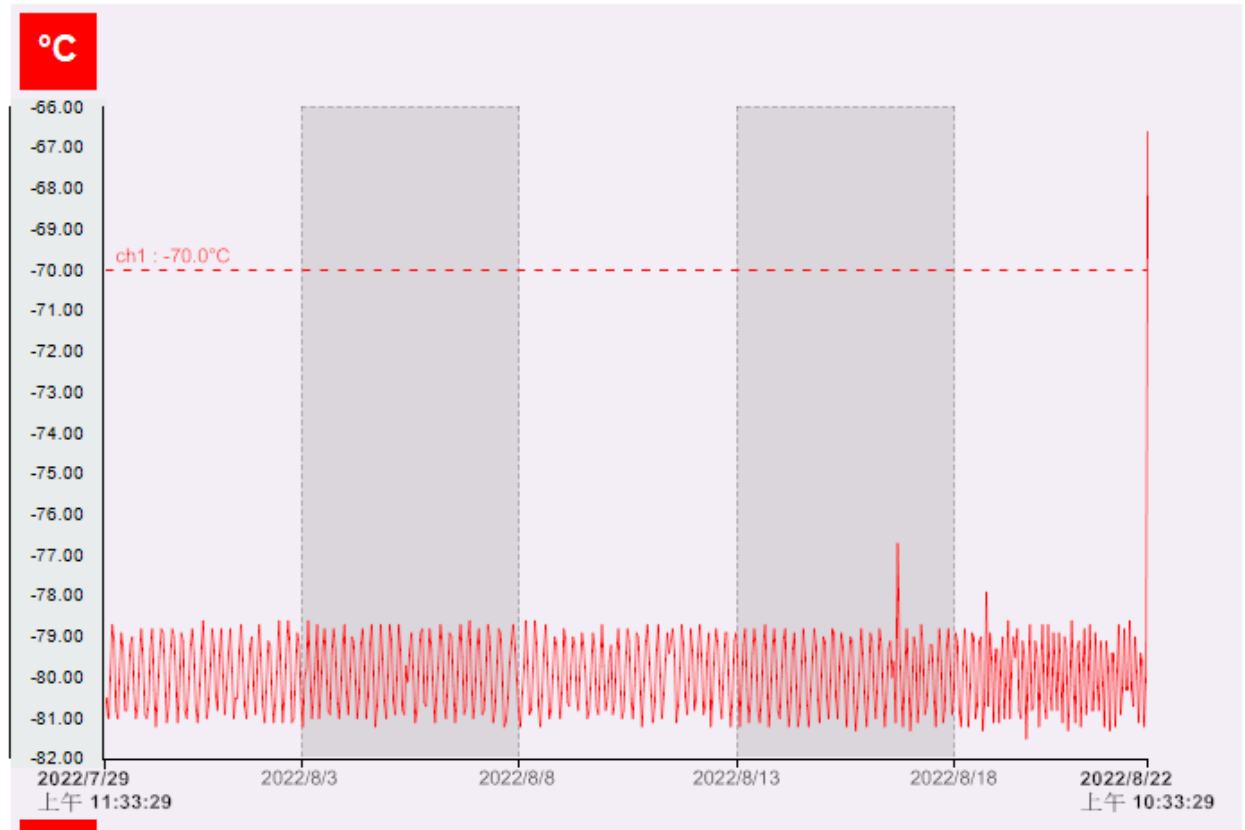

Comment: 於2022年8月22日10:00放冰寶之後由於溫差較大而暫時升溫，但仍低於-60°C，符合目前放置藥品之保存溫度。 9

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 22, Aug 2022 ~ 31, Aug 2022



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.4 -72.1 -79.89 1.14 -79.68

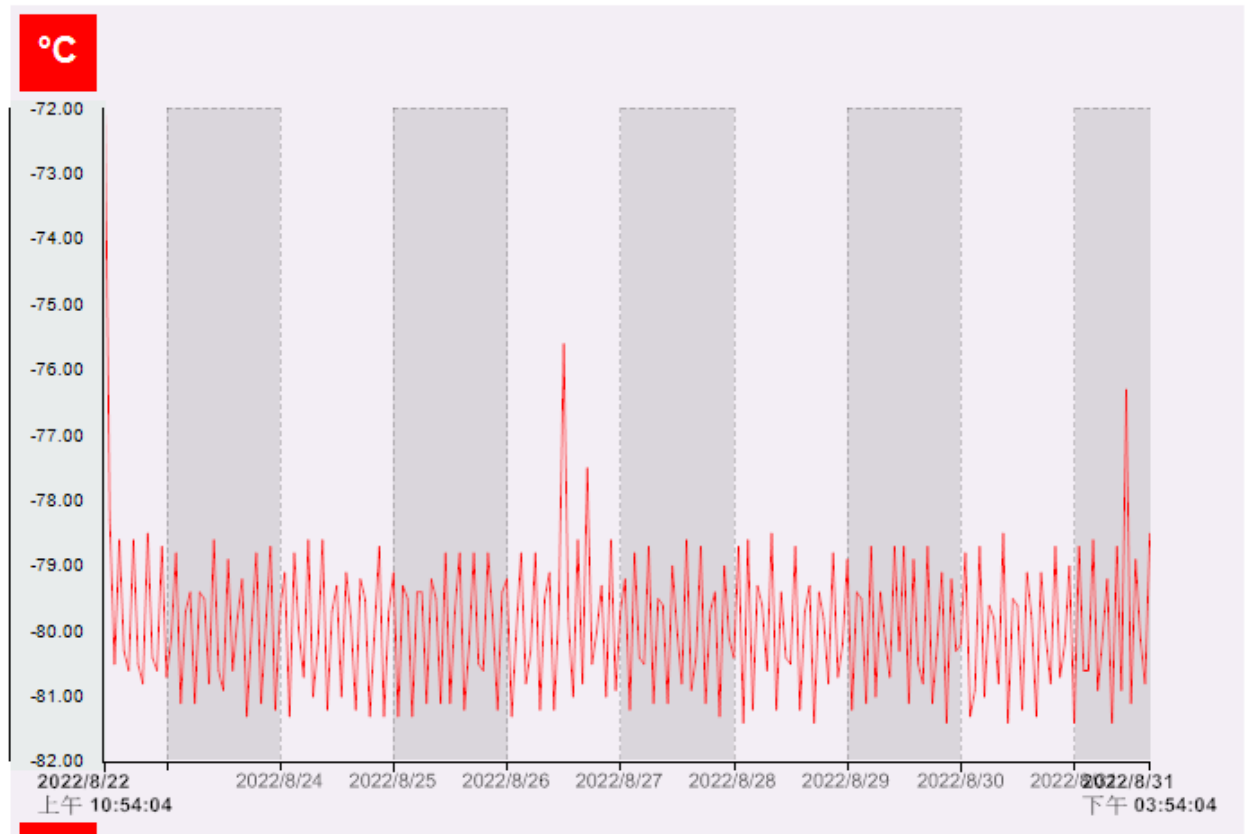

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 31, Aug 2022 ~ 30, Sep 2022



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.5 -75.2 -80.17 0.85 -80.07

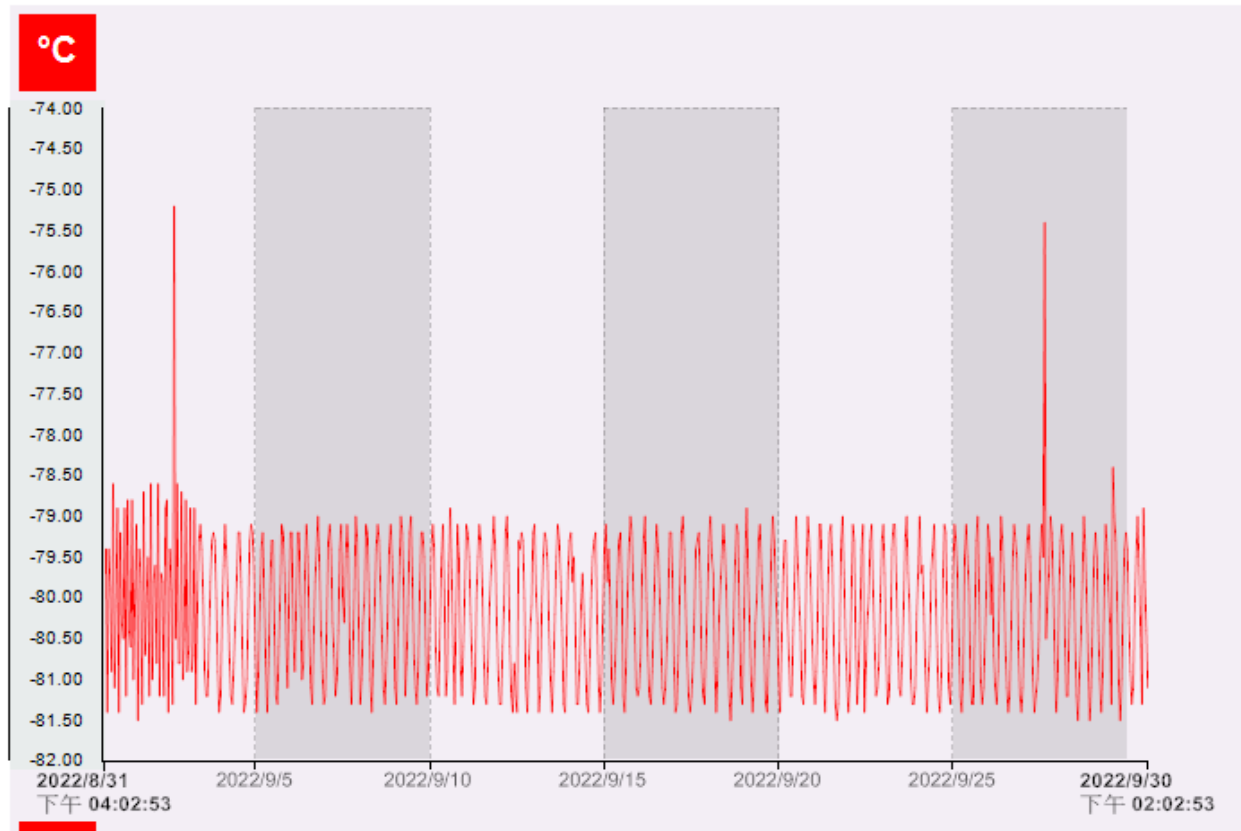

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 30, Sep 2022 ~ 28, Oct 2022



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.5 -74.8 -80.05 0.85 -79.95

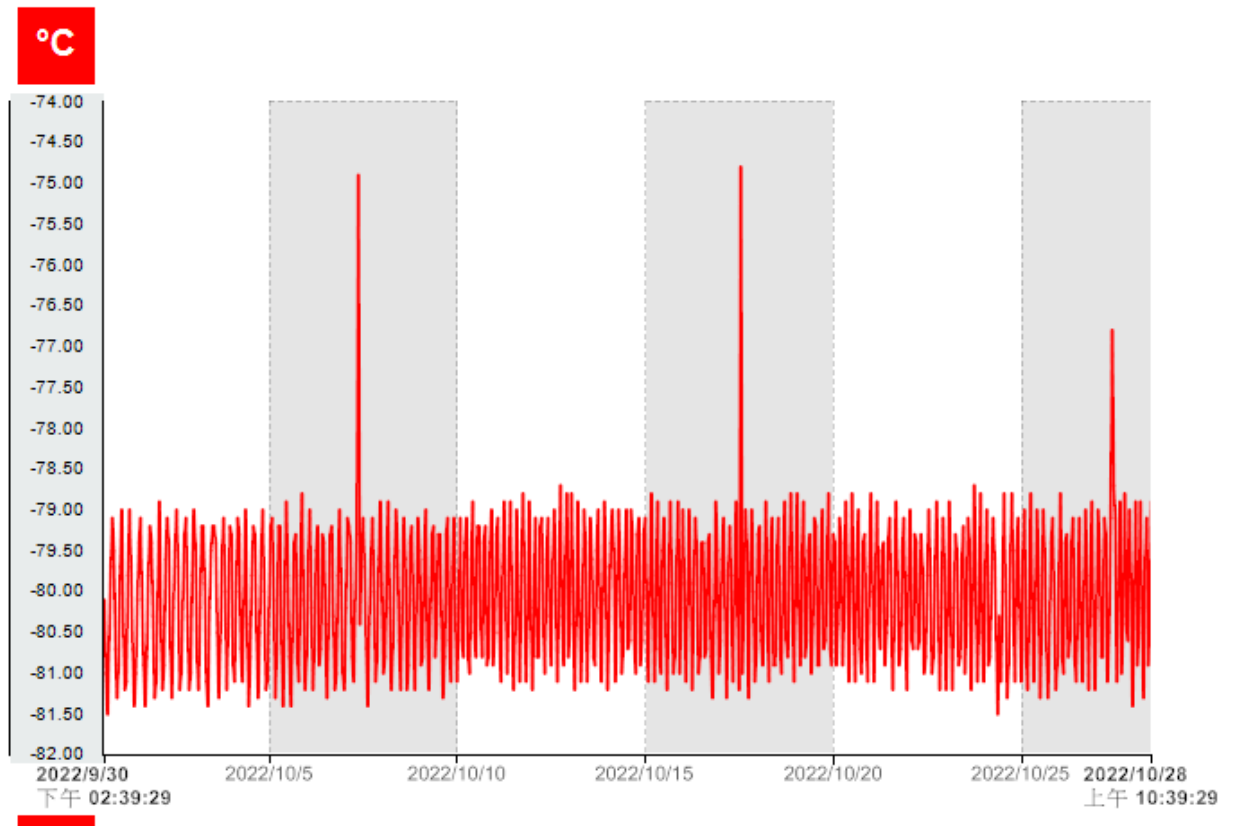

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 28, Oct 2022 ~ 30, Nov 2022



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.4 -76.9 -80.00 0.86 -79.91

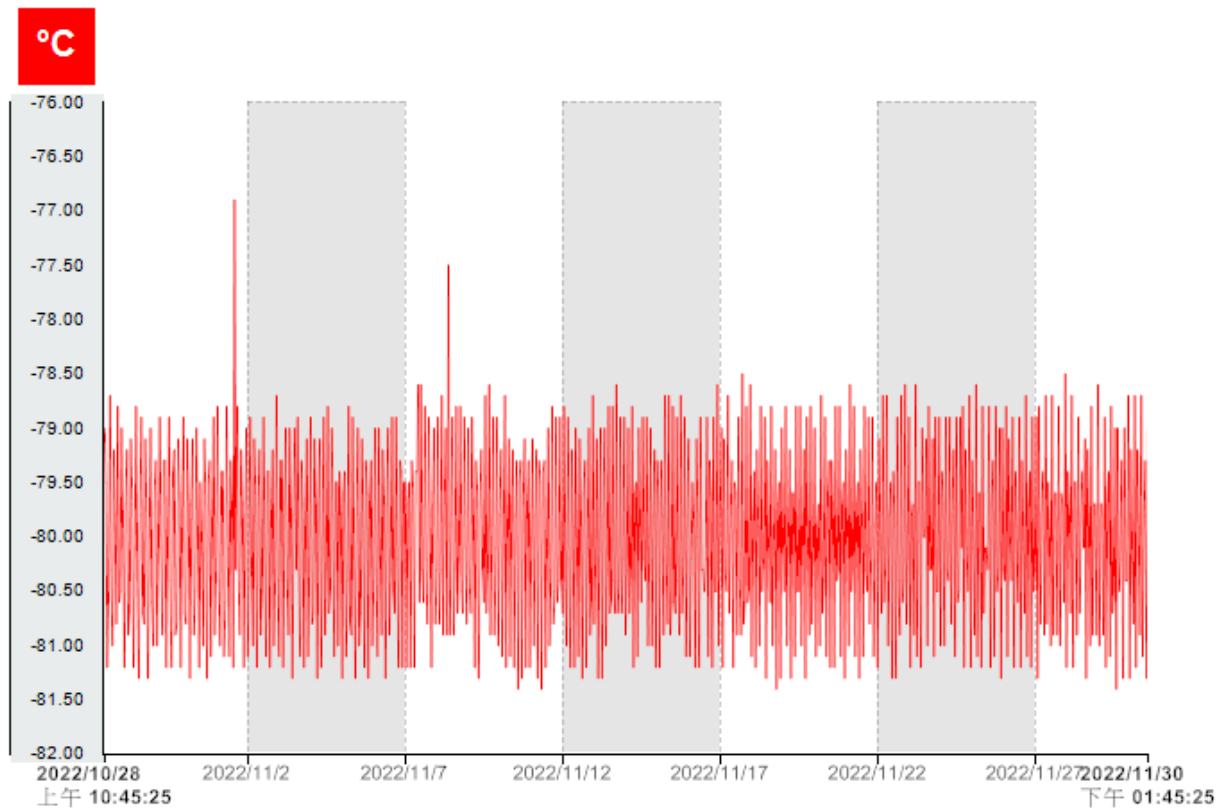

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80±10 °C

DATE : 30, Nov 2022 ~ 03, Jan 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.5 -78.1 -80.00 0.87 -79.91

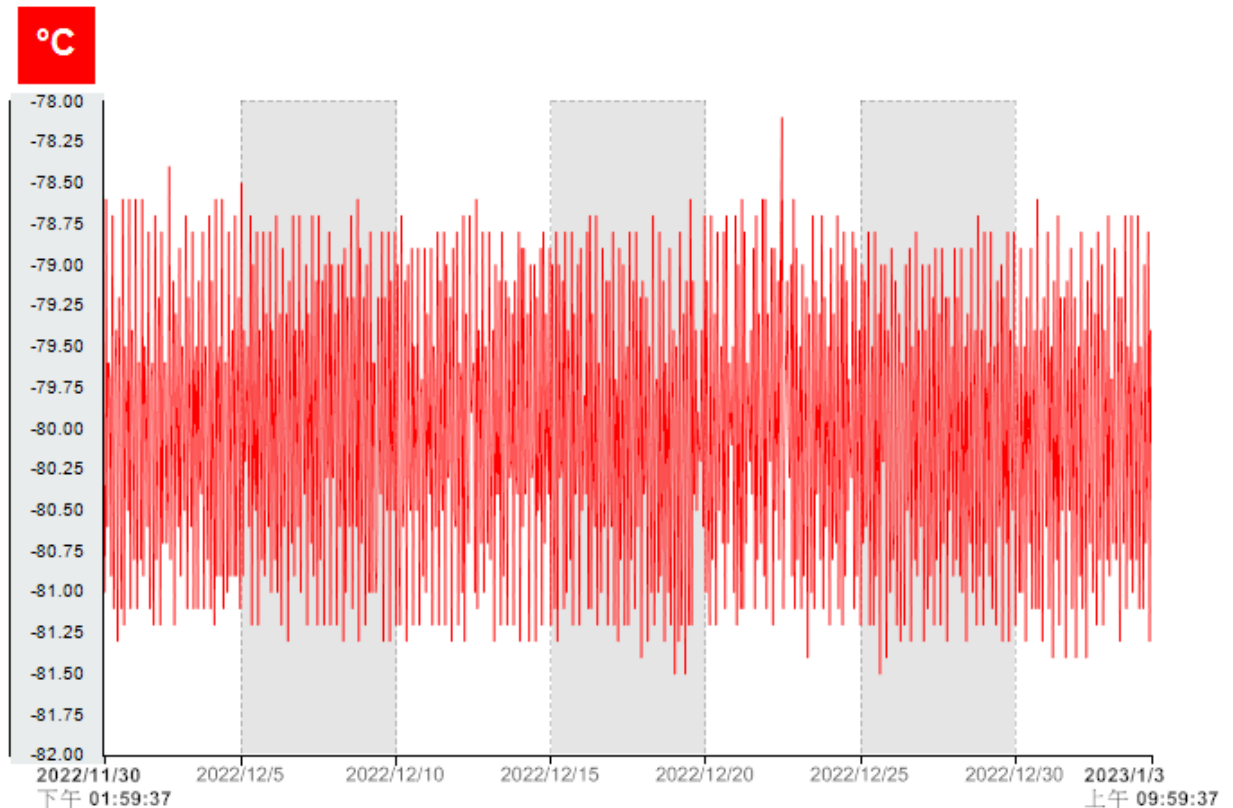

Comment: