

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Dec 2021 ~ 25, Jan 2022



KIMO 2K190616069

— v1 [°C]				
Min	Max	Avg	Sd	MKT
3.0	5.5	3.56	0.23	3.57

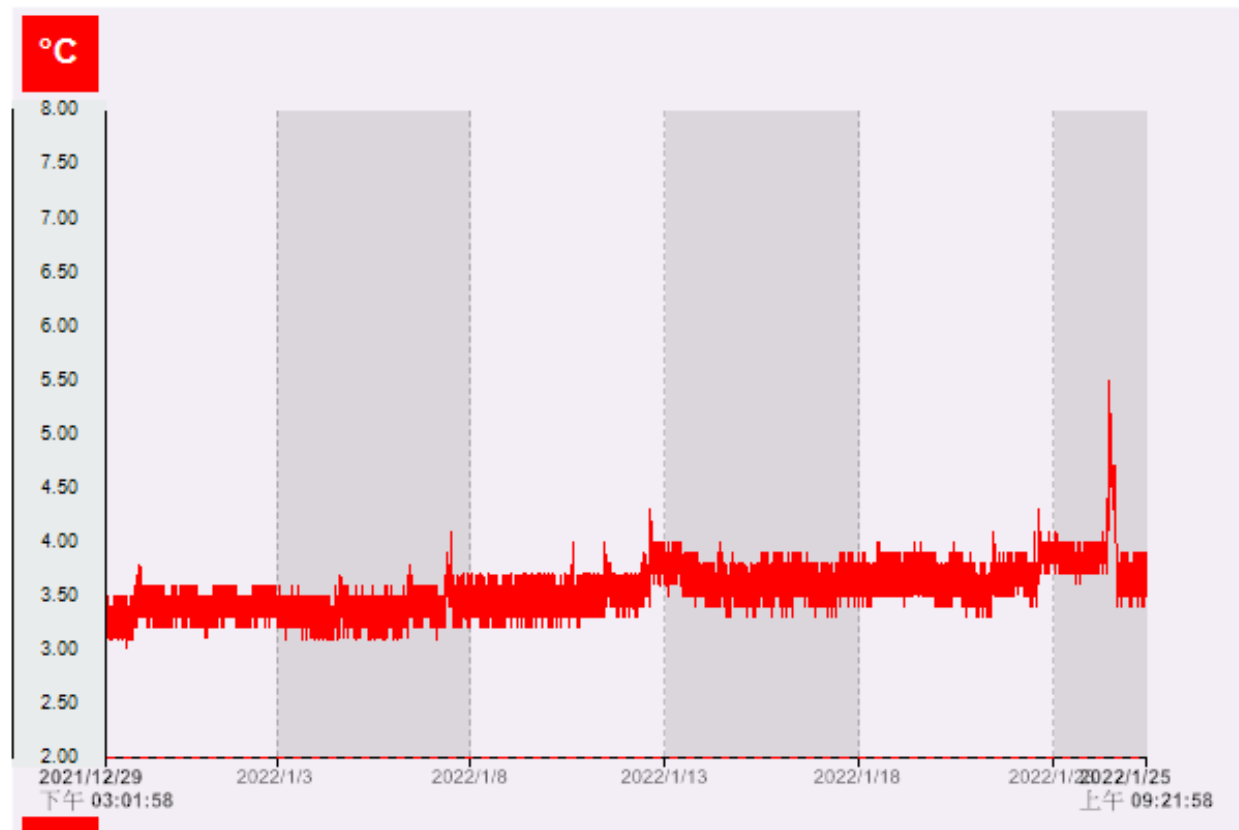

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 25, Jan 2022 ~ 24, Feb 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.2	5.6	4.18	0.45	4.19

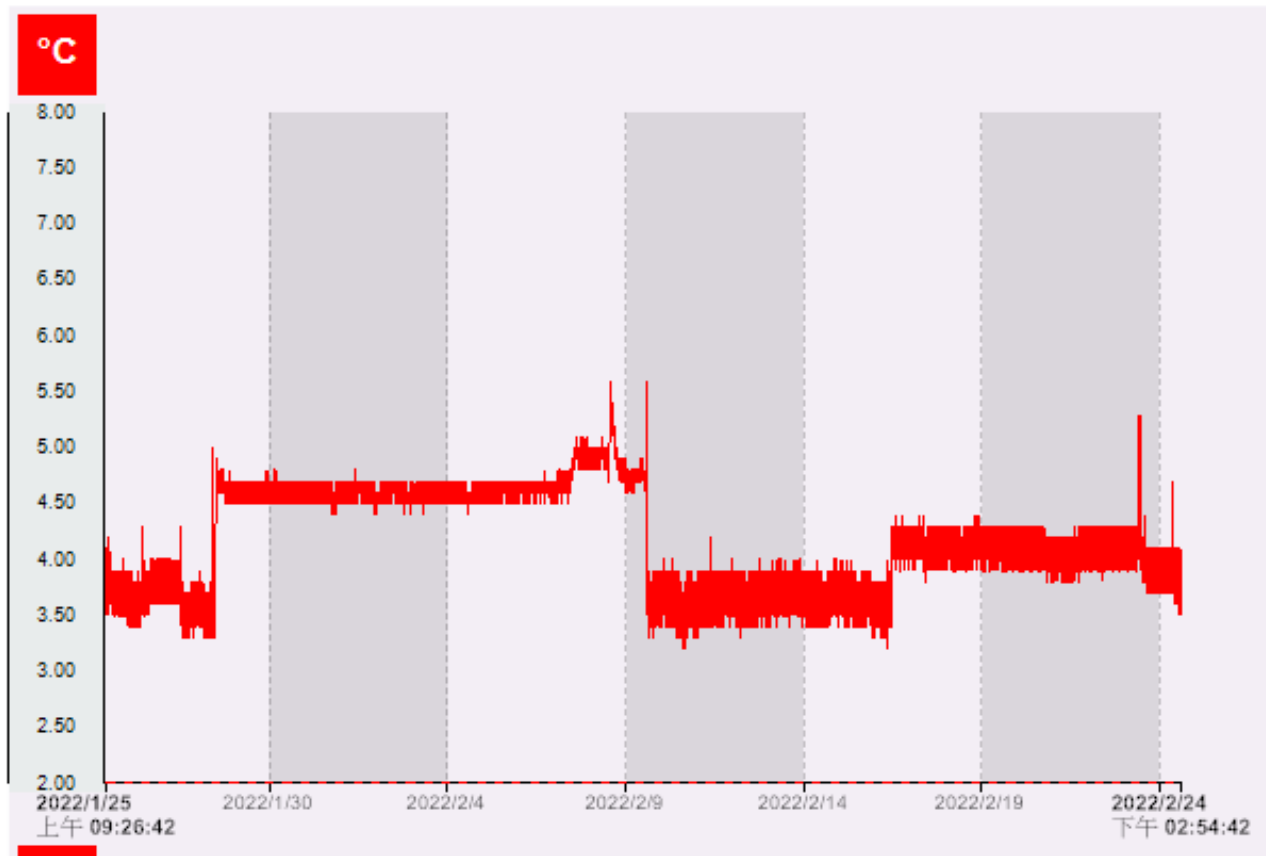

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KT220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 24, Feb 2022 ~ 31, Mar 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	6.1	4.08	0.24	4.08

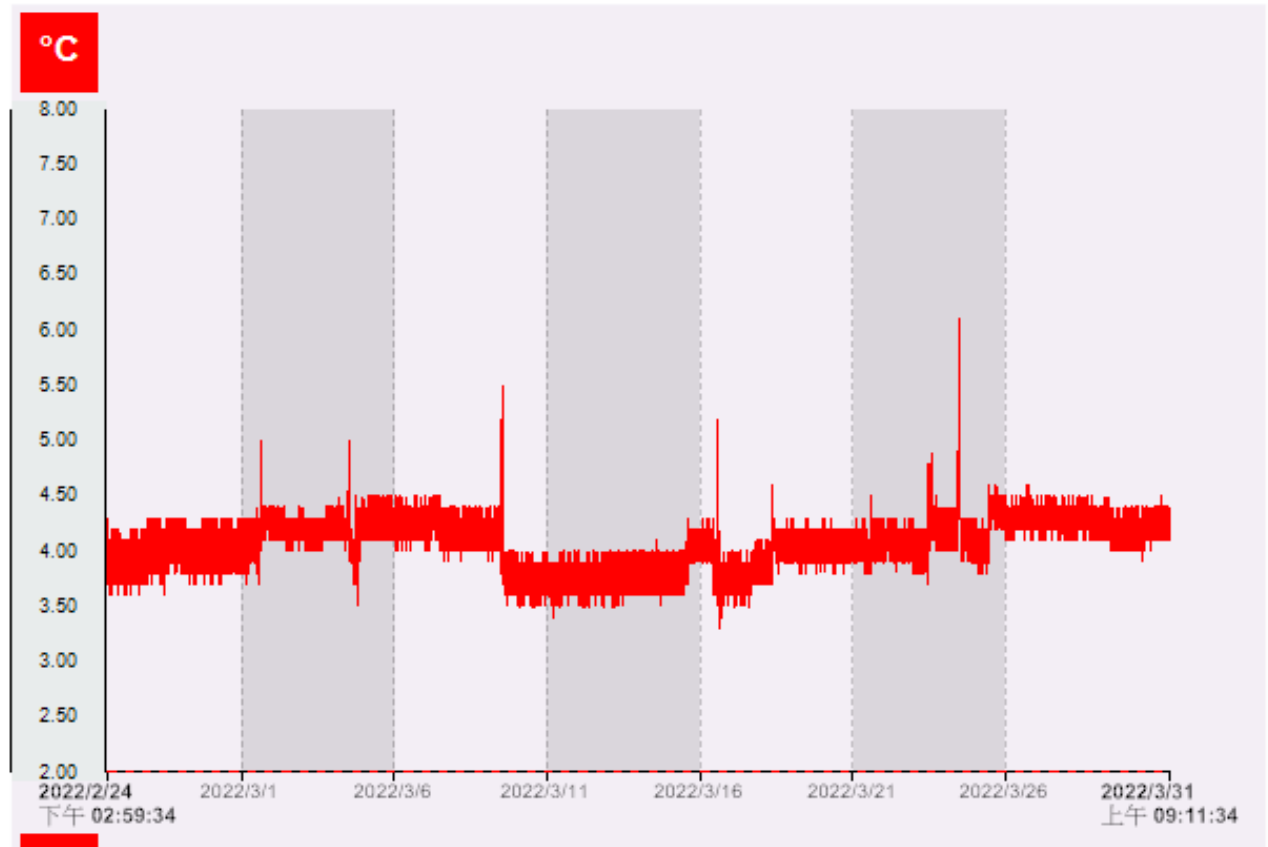

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KT20-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Mar 2022 ~ 29, Apr 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.7	5.1	4.24	0.17	4.25

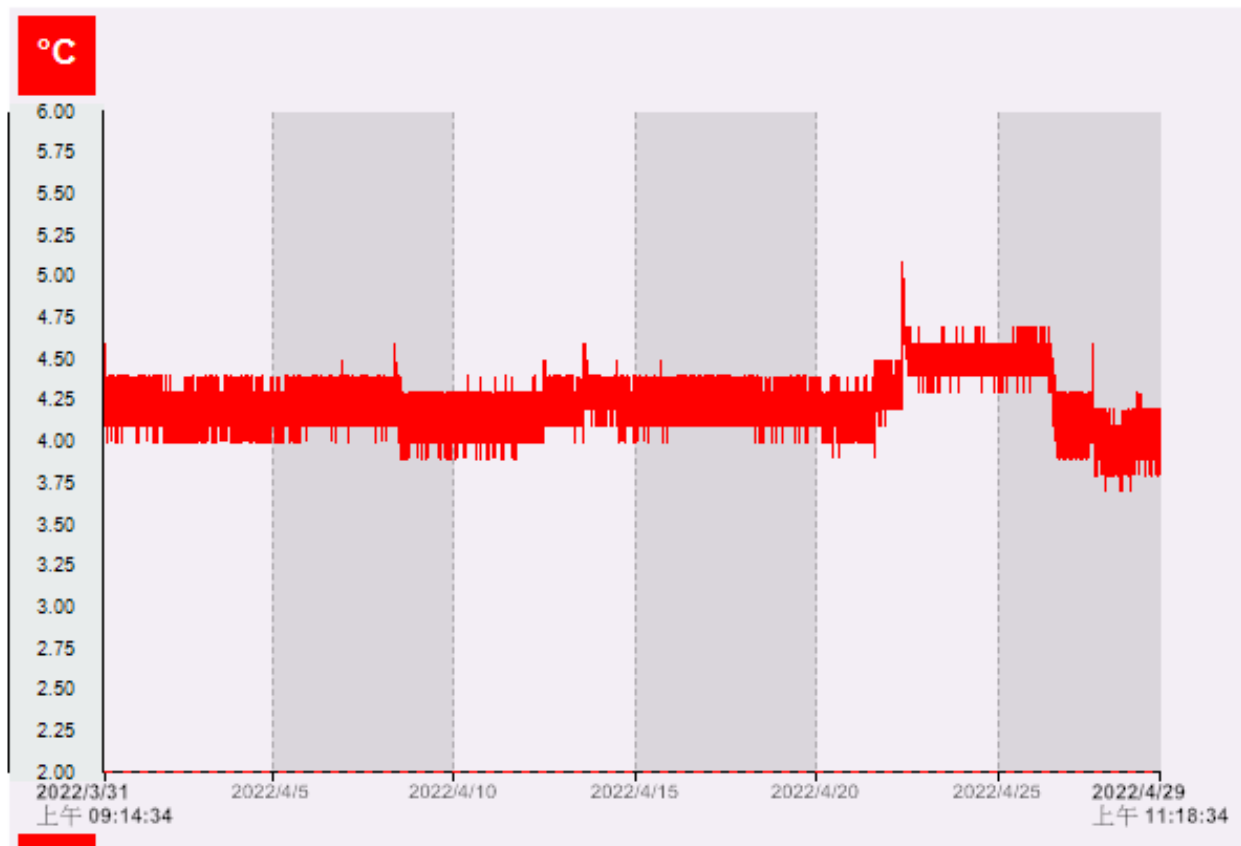

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Apr 2022 ~ 30, May 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.6	5.5	4.11	0.45	4.12

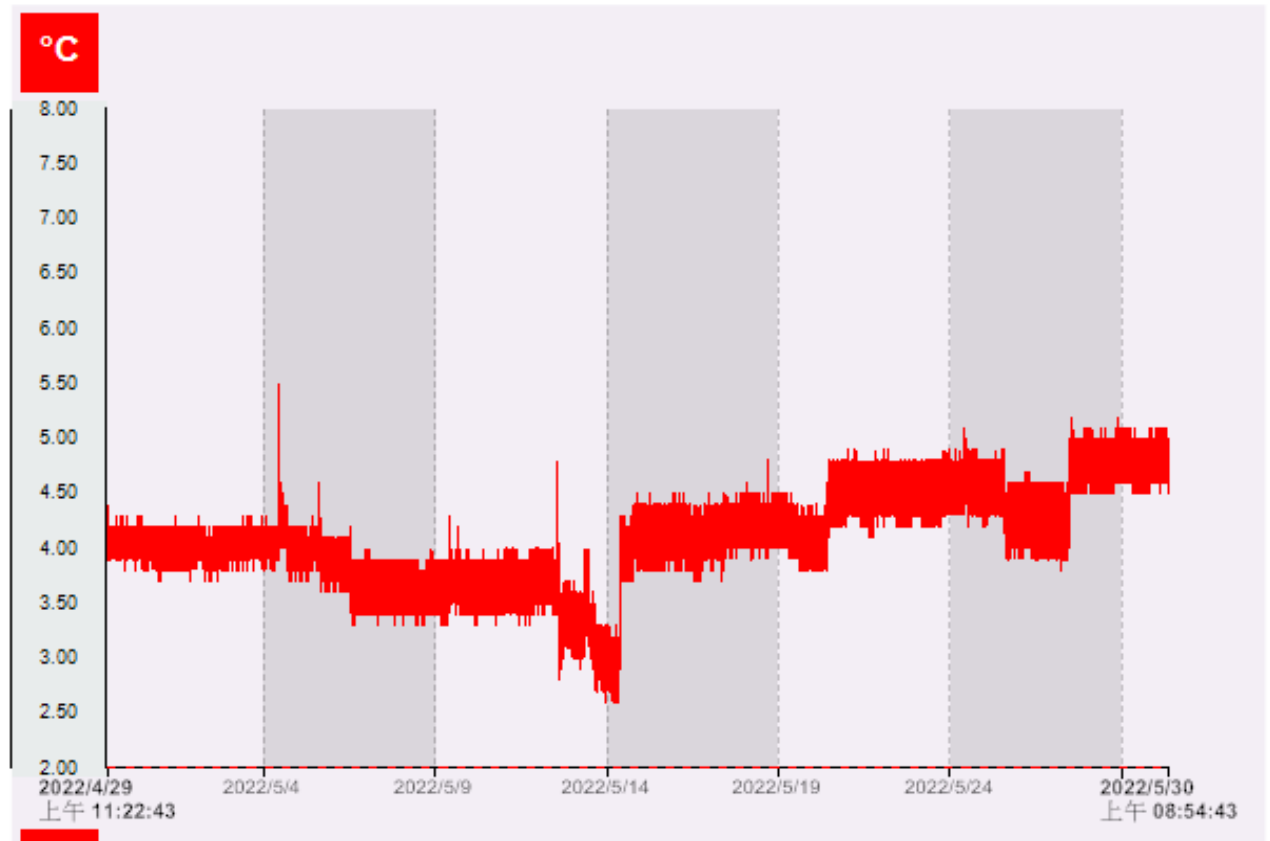

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT 220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, May 2022 ~ 28, Jun 2022



KIMO 2K190616069

— v1 [°C]				
Min	Max	Avg	Sd	MKT
4.0	6.2	4.85	0.25	4.85

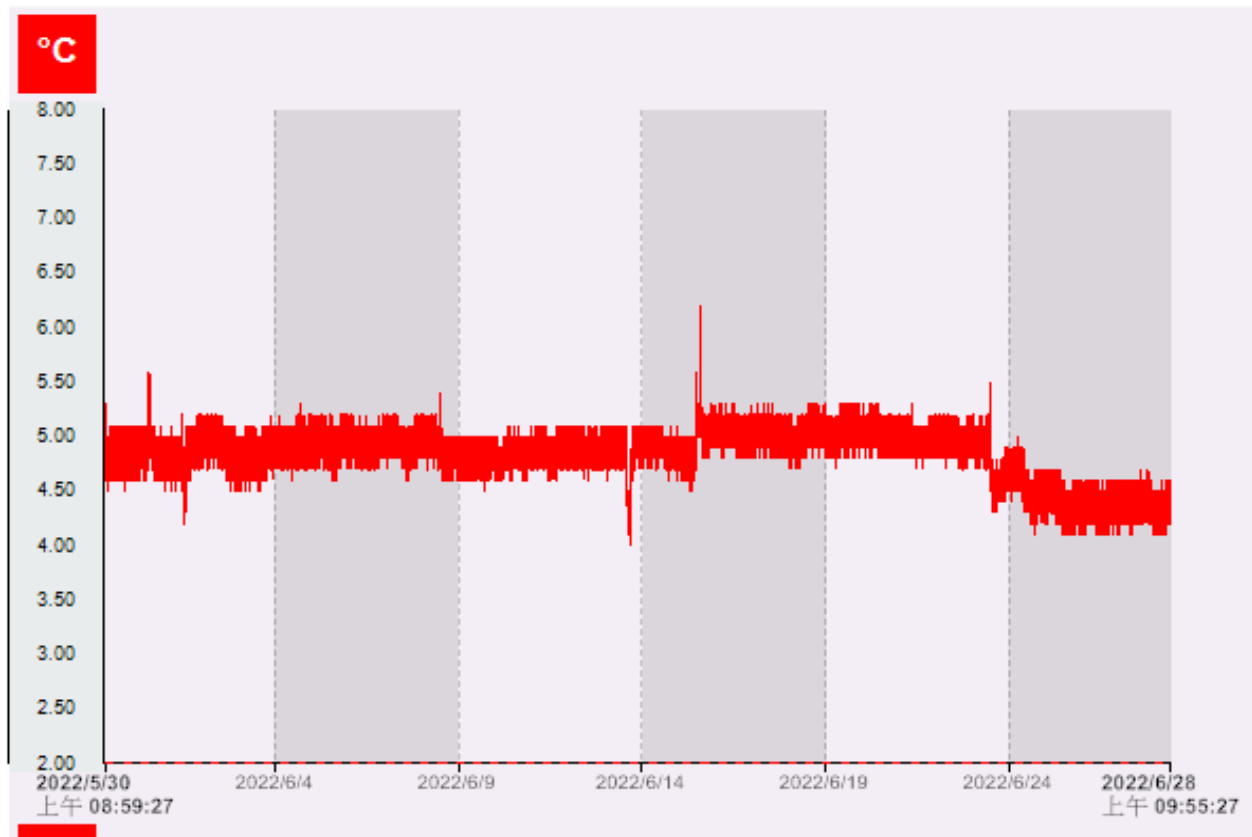

Comment :

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-310; Serial No.: 1305 1668; Channel No.: 1

REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 28, Jun 2022 ~ 21, Jul 2022

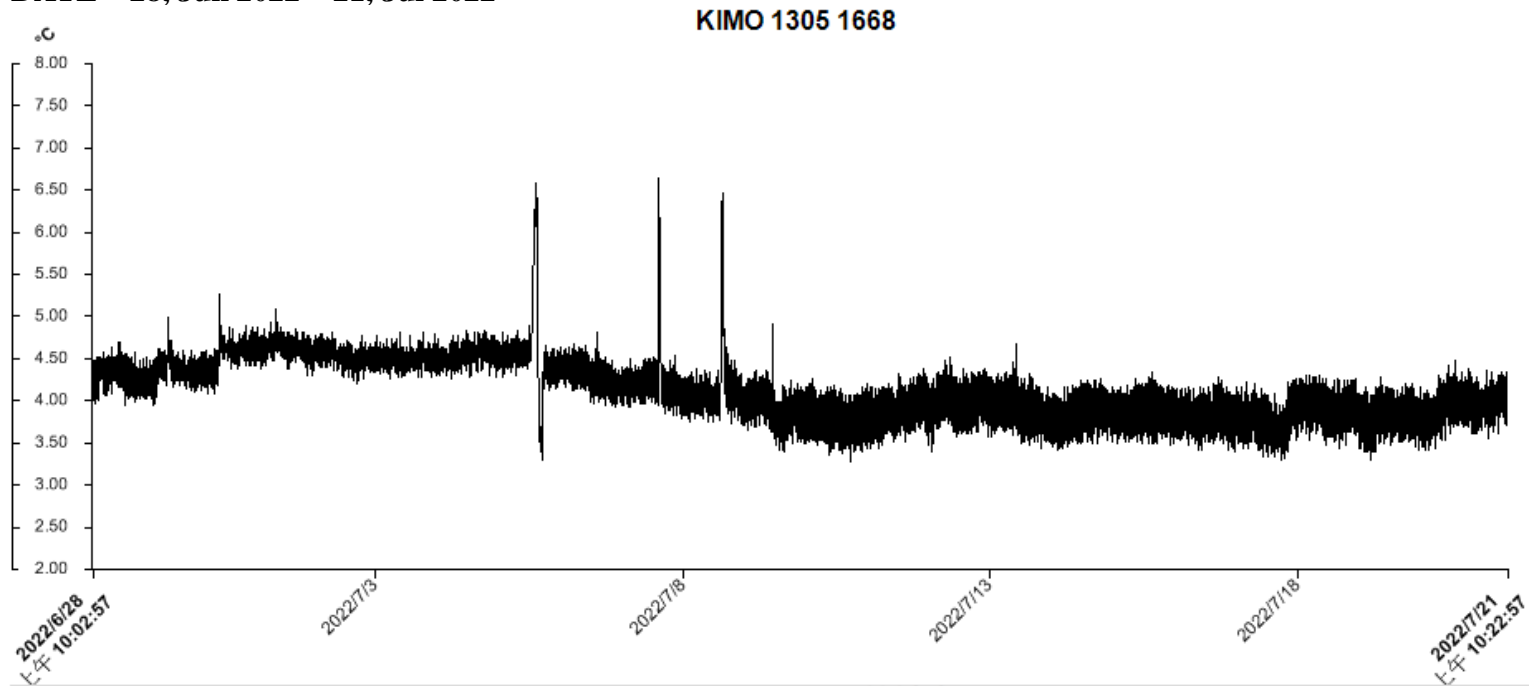

統計表

	#1
最小 T	3.27
最小 t	3.27
最大值 T	6.65
最大值 t	6.65
平均值 T	4.141
平均值 t	4.141
標準偏差 T	0.374
標準偏差 t	0.374
MKT T	4.14
MKT t	4.14

T: 整個週期
t: 顯示週期

Comment: 本溫度記錄器(2K190616069)於2022年6月28日送校，期間以備品溫度記錄器(1305 1668)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1

REFRIGERATOR TEMPERATURE RANGE : 2-8°C


DATE : 21, Jul 2022 ~ 29, Jul 2022



KIMO 2K190616069

— v1 [°C]

Min	Max	Avg	Sd	MKT
3.9	6.8	4.68	0.38	4.68

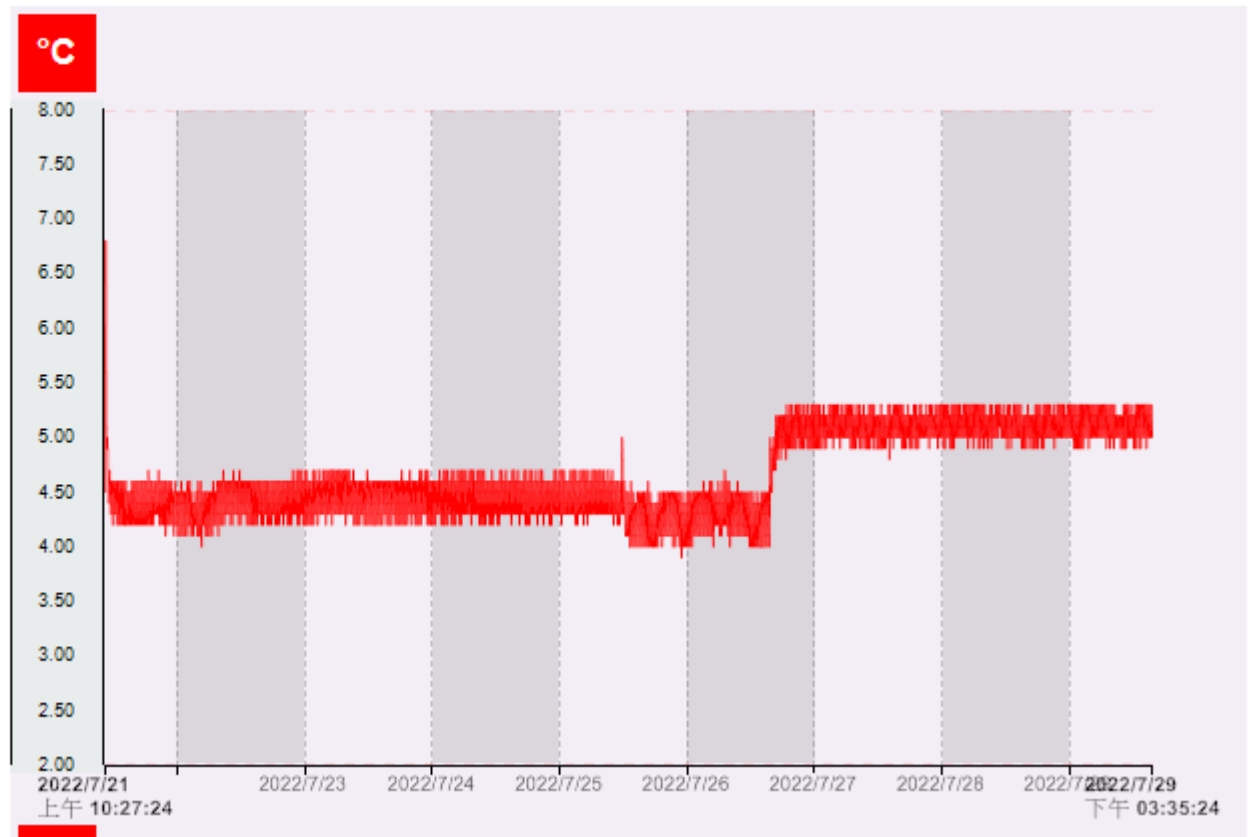

Comment: 本溫度記錄器(2K190616069)於2022年7月11日完成校正。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, Jul 2022 ~ 31, Aug 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.7	5.8	4.65	0.36	4.65

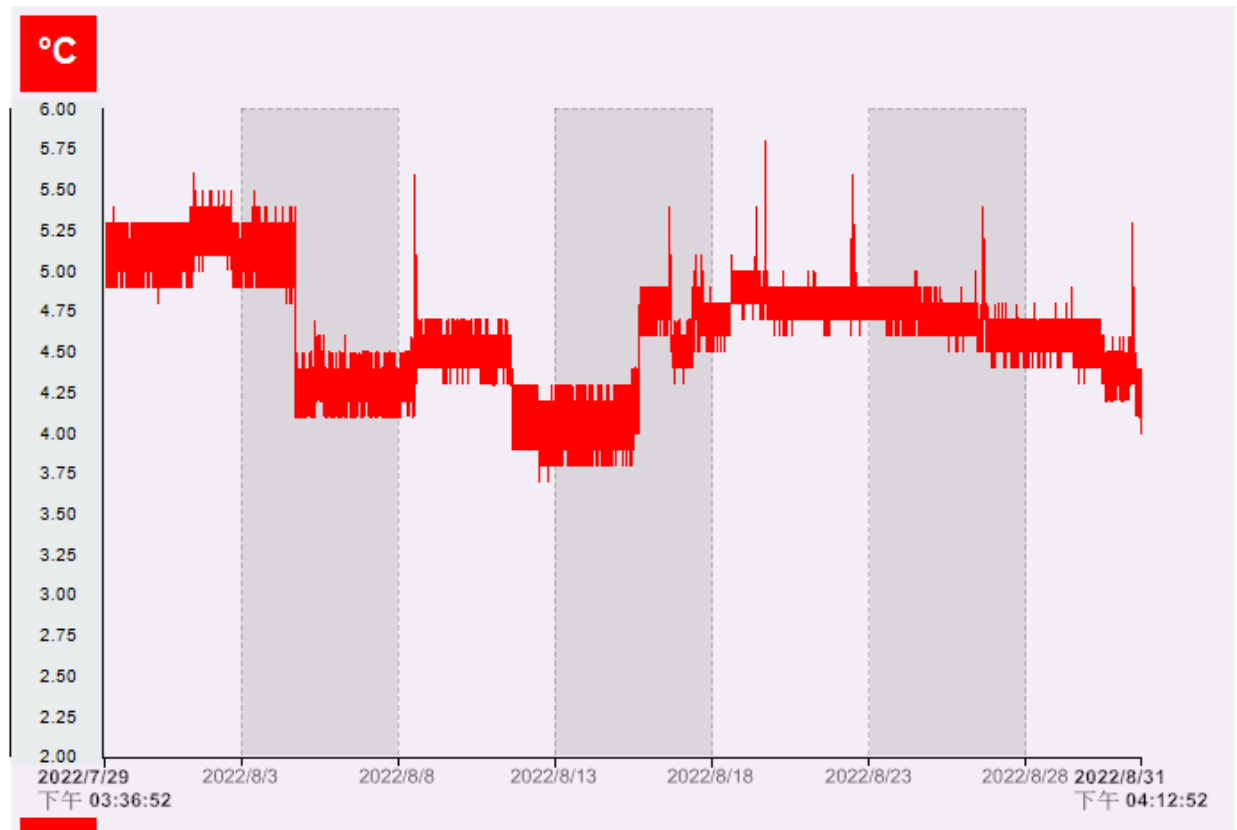

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Aug 2022 ~ 30, Sep 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.9	6.4	4.37	0.16	4.37

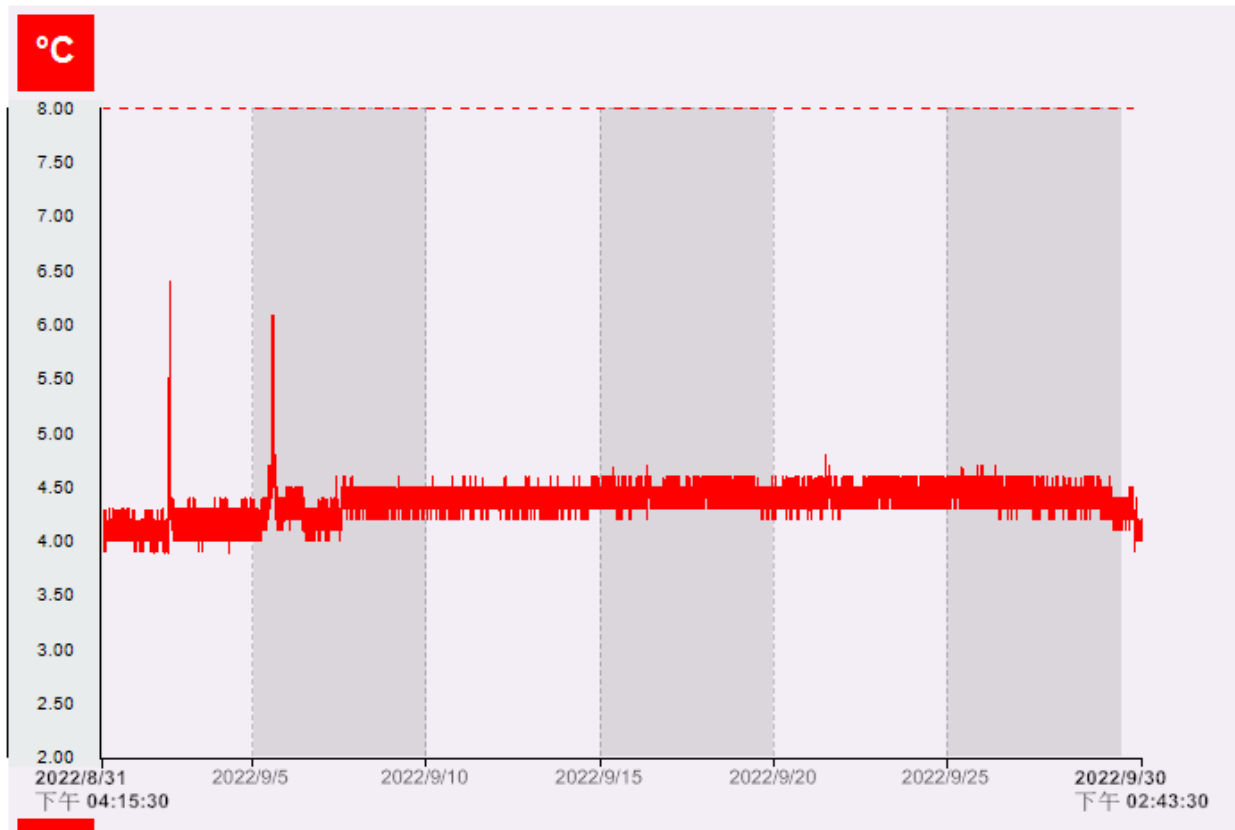

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Sep 2022 ~ 28, Oct 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.7	5.0	4.20	0.20	4.20

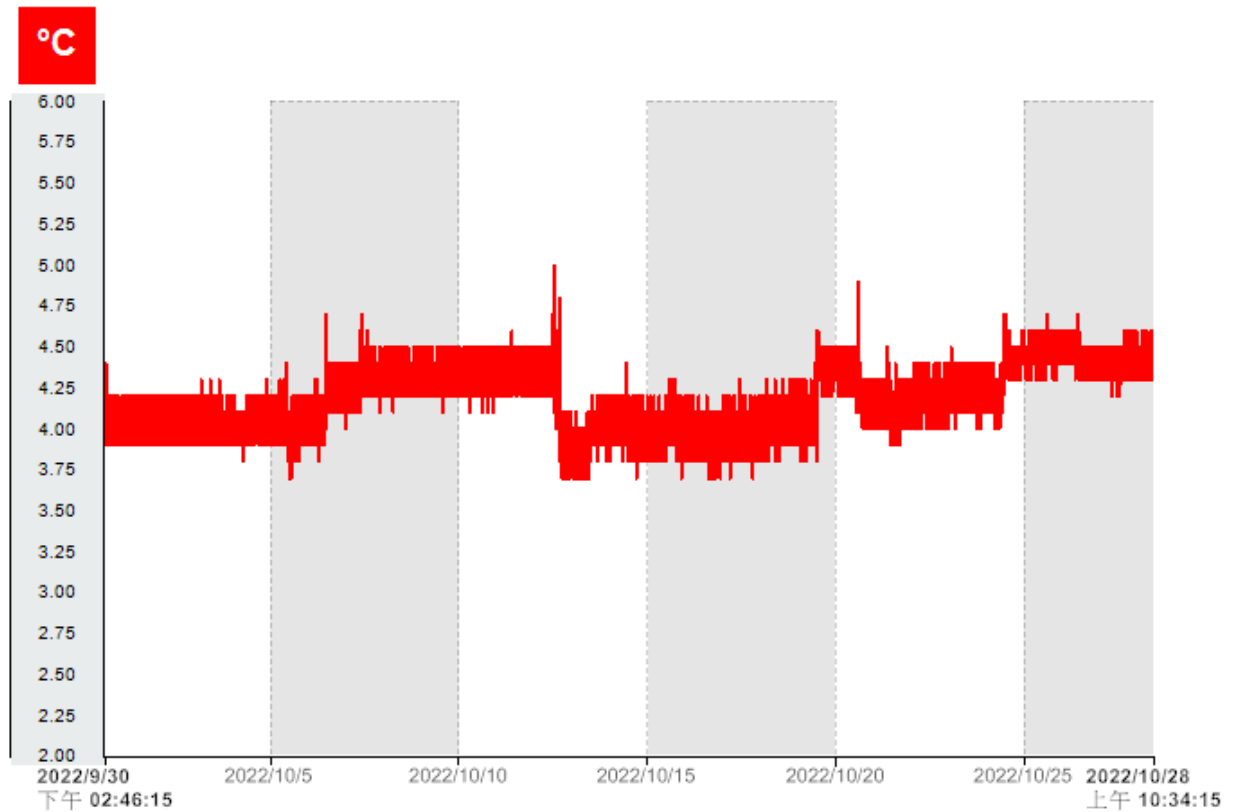

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 28, Oct 2022 ~ 30, Nov 2022



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
4.0	6.0	4.50	0.13	4.50

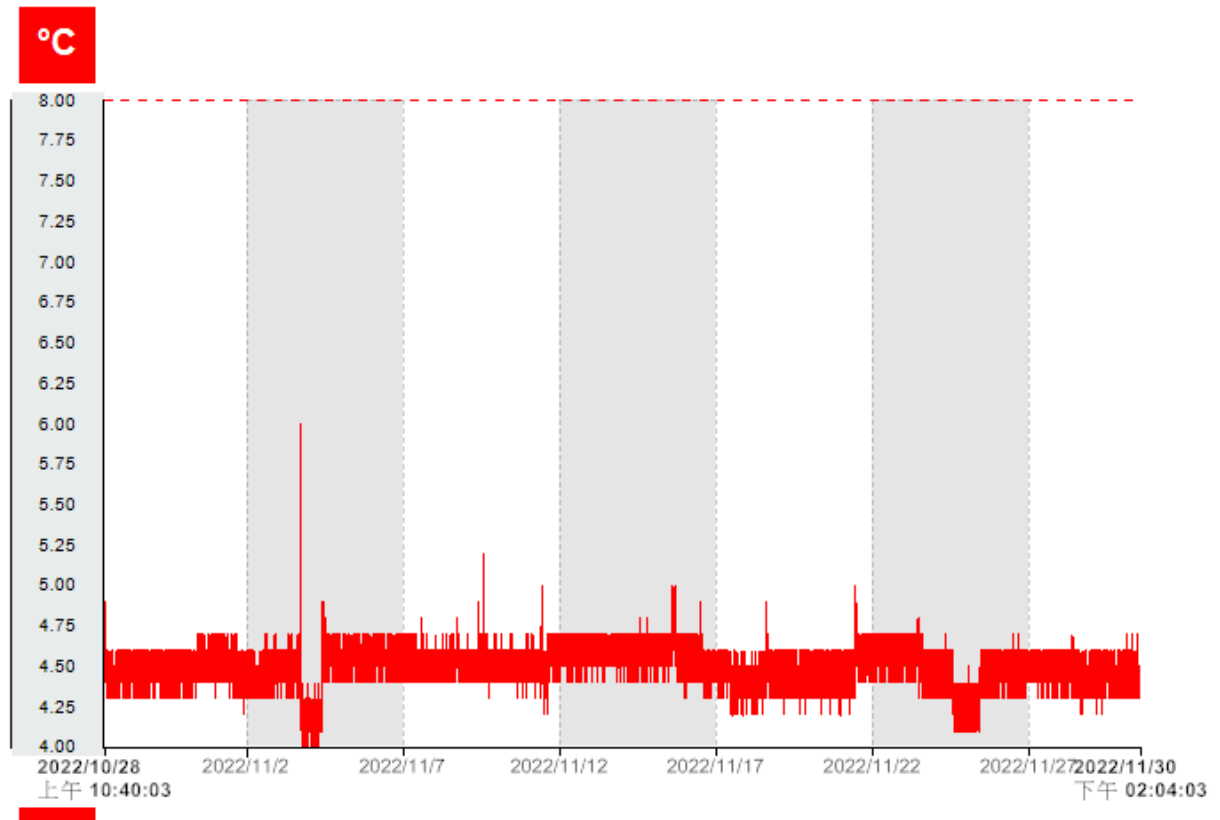

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1

REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Nov 2022 ~ 03, Jan 2023



KIMO 2K190616069

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.2	5.8	4.20	0.41	4.21



Comment: