

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 03, Jan 2023 ~ 30, Jan 2023

Instrument name: Testo 176T2		2023/1/30 上午 11:00:10			Page 1/1
Start time: 2023/1/3 上午 11:22:32		Minimum	Maximum	Mean value	Limit values
End time: 2023/1/30 上午 10:22:32	40505446 [°C]	-74.12	-71.68	-73.000	-80.0/-60.0
Measurement channels: 1					
Measured values: 648					
SN 40505446					

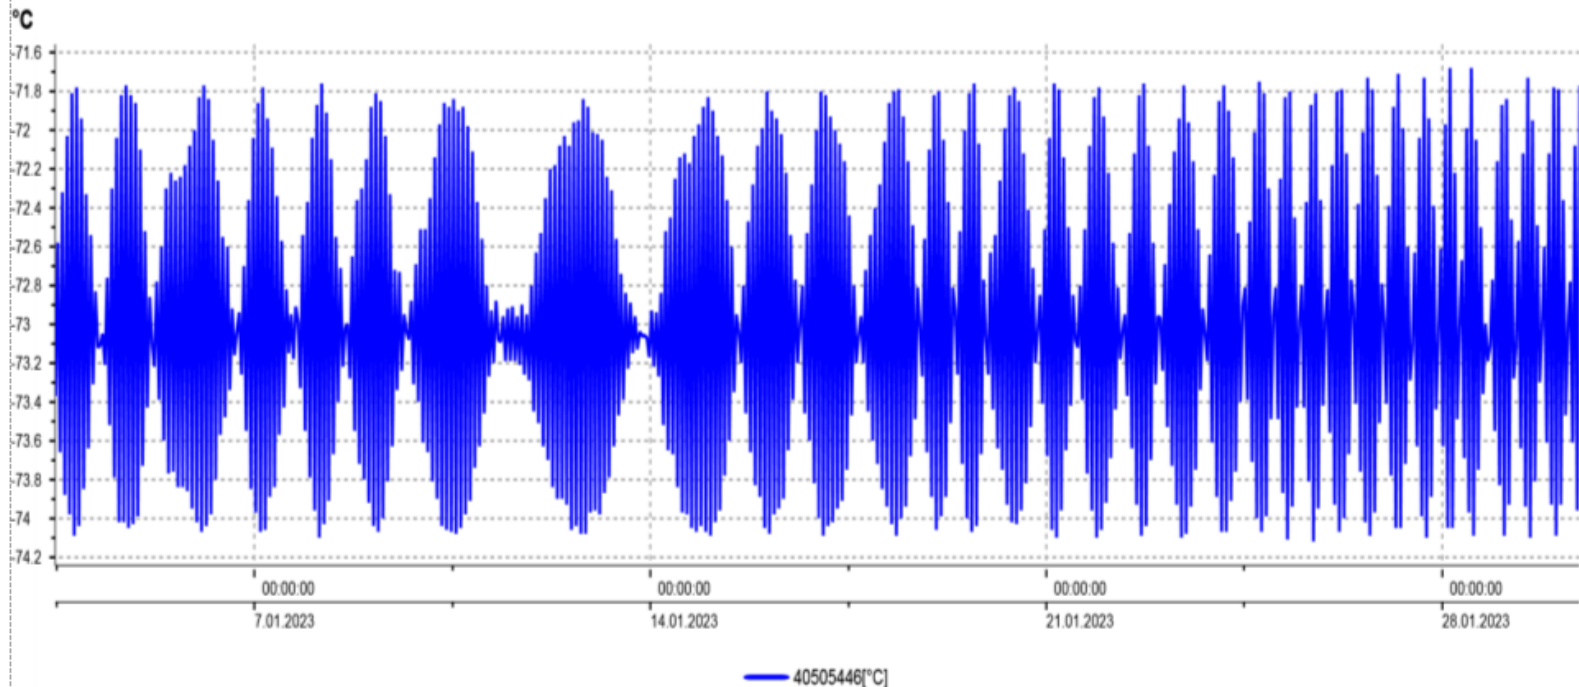

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 30, Jan 2023 ~ 01, Mar 2023

Instrument name: Testo 176T2		2023/3/1 上午 11:12:50			Page 1/1
Start time: 2023/1/30 上午 10:57:12		Minimum	Maximum	Mean value	Limit values
End time: 2023/3/1 上午 10:57:12	40505446 [°C]	-74.09	-71.37	-72.558	-80.0/-60.0
Measurement channels: 1					
Measured values: 721					
SN 40505446					

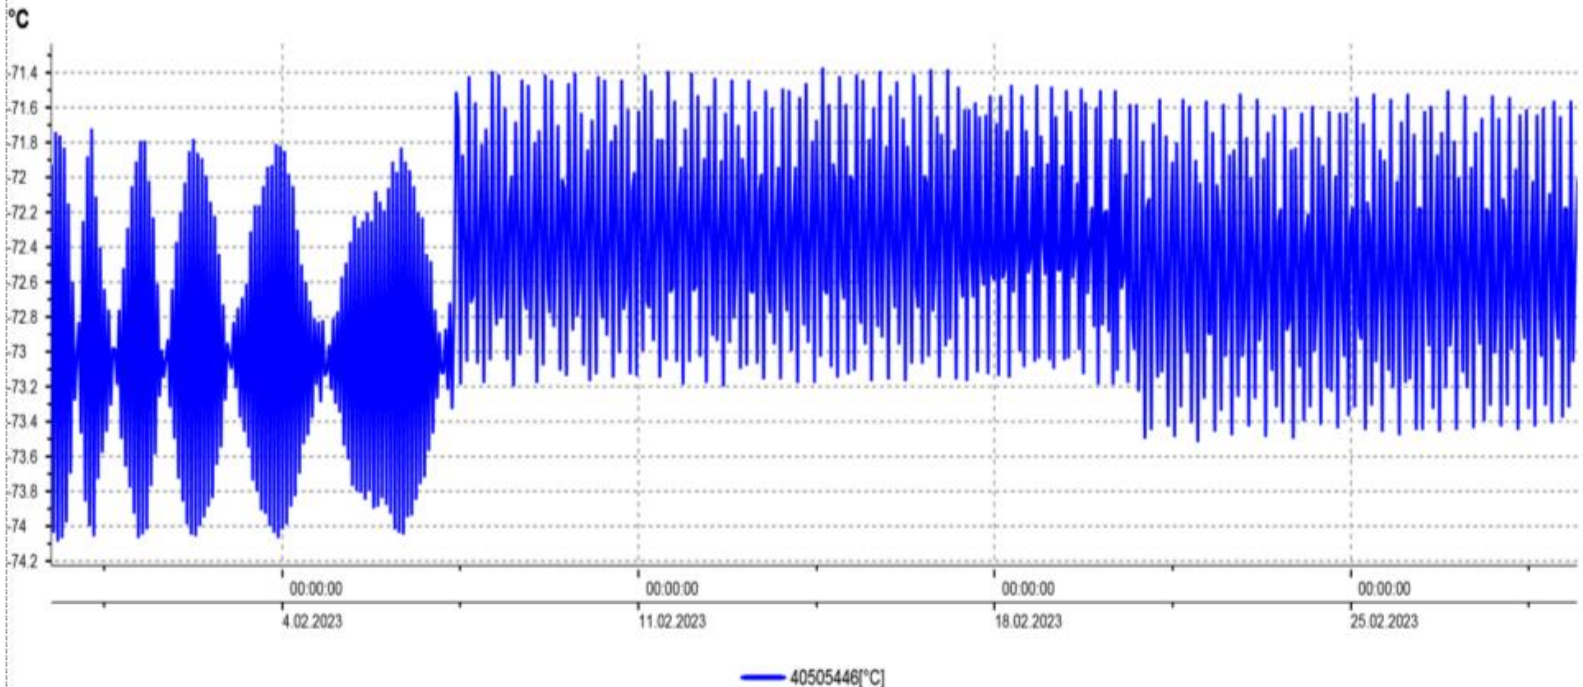

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 01, Mar 2023 ~ 31, Mar 2023

Instrument name: Testo 176T2		2023/3/31 上午 11:01:42			Page 1/1
Start time: 2023/3/1 上午 11:10:39		Minimum	Maximum	Mean value	Limit values
End time: 2023/3/31 上午 09:10:39	40505446 [°C]	-73.49	-71.47	-72.481	-80.0/-60.0
Measurement channels: 1					
Measured values: 719					
SN 40505446					

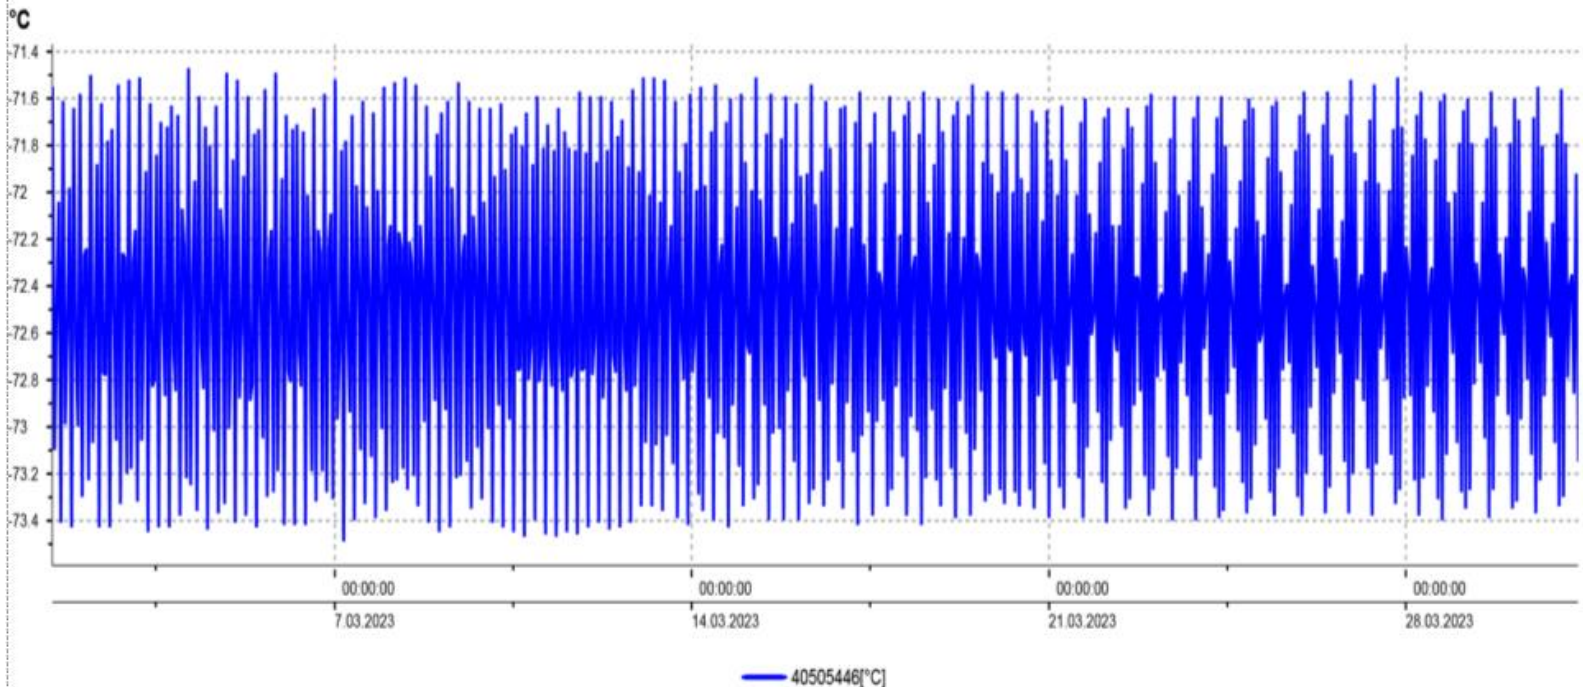

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31, Mar 2023 ~ 28, Apr 2023

Instrument name: Testo 176T2		2023/5/2 上午 10:10:56			Page 1/1
Start time: 2023/3/31 上午 09:53:48		Minimum	Maximum	Mean value	Limit values
End time: 2023/4/28 下午 03:53:48	40505446 [°C]	-73.42	-71.52	-72.459	-80.0/-60.0
Measurement channels: 1					
Measured values: 679					
SN 40505446					

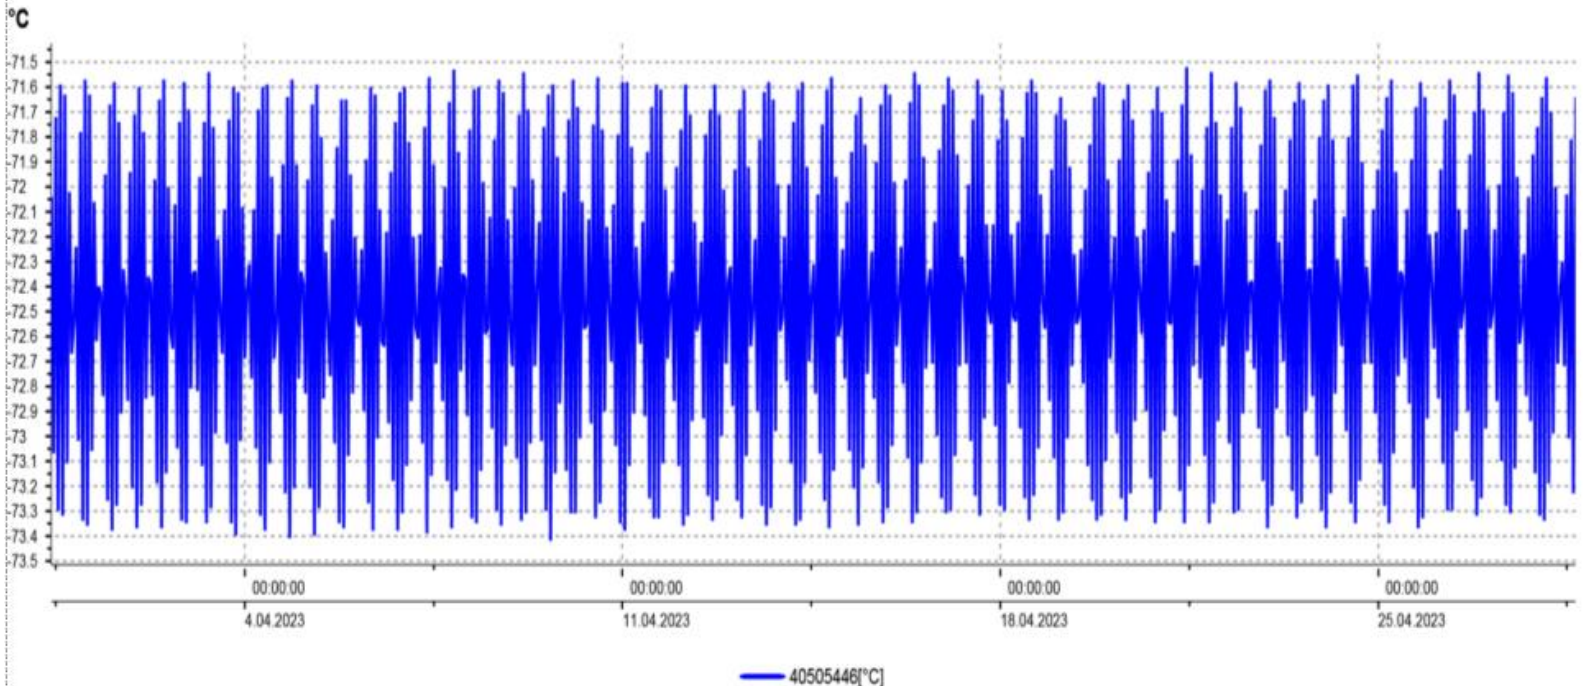

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 28, Apr 2023 ~ 29, May 2023

Instrument name: Testo 176T2		2023/5/29 上午 10:19:19			Page 1/1
Start time: 2023/4/28 下午 04:08:09		Minimum	Maximum	Mean value	Limit values
End time: 2023/5/29 上午 10:08:09	40505446 [°C]	-73.36	-71.55	-72.446	-80.0/-60.0
Measurement channels: 1					
Measured values: 739					
SN 40505446					

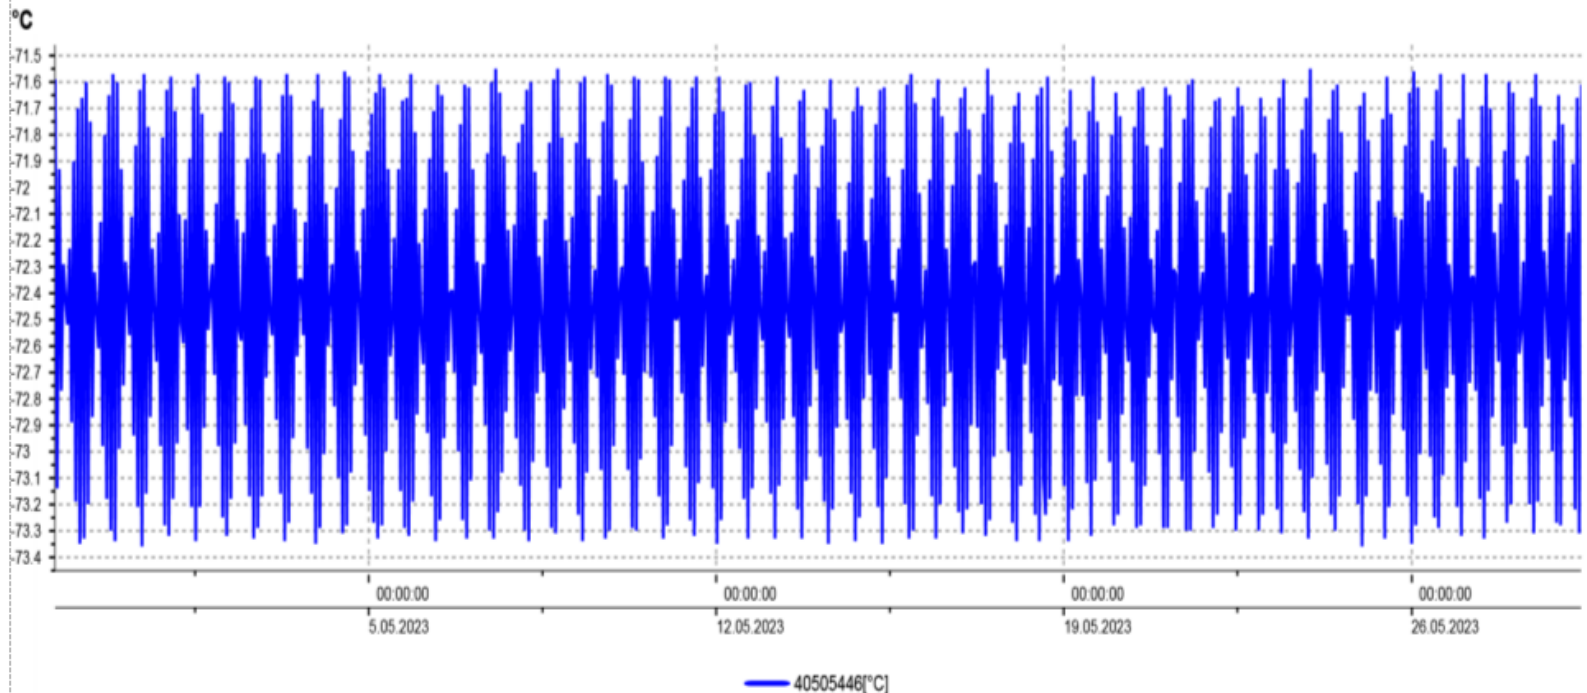

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 29, May 2023 ~ 30, Jun 2023

Instrument name: Testo 176T2		2023/6/30 下午 02:02:59			Page 1/1
Start time: 2023/5/29 上午 10:17:00		Minimum	Maximum	Mean value	Limit values
End time: 2023/6/30 上午 10:17:00	40505446 [°C]	-73.35	-71.57	-72.447	-80.0/-60.0
Measurement channels: 1					
Measured values: 769					
SN 40505446					

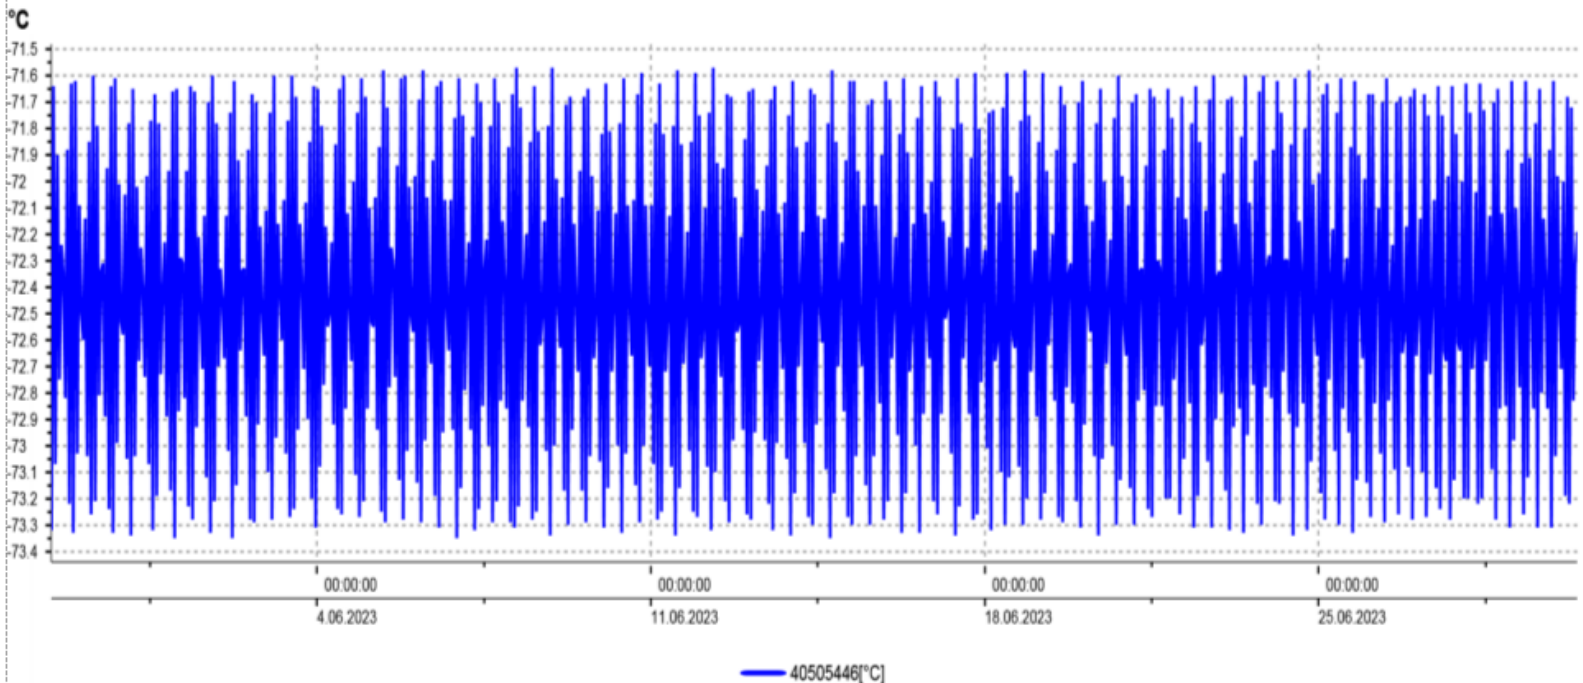

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 30, Jun 2023 ~ 31, Jul 2023

Instrument name: Testo 176T2		2023/7/31 下午 04:41:32			Page 1/1
Start time: 2023/6/30 上午 11:09:23		Minimum	Maximum	Mean value	Limit values
End time: 2023/7/31 上午 09:09:23	40505446 [°C]	-73.33	-71.61	-72.442	-80.0/-60.0
Measurement channels: 1					
Measured values: 743					
SN 40505446					

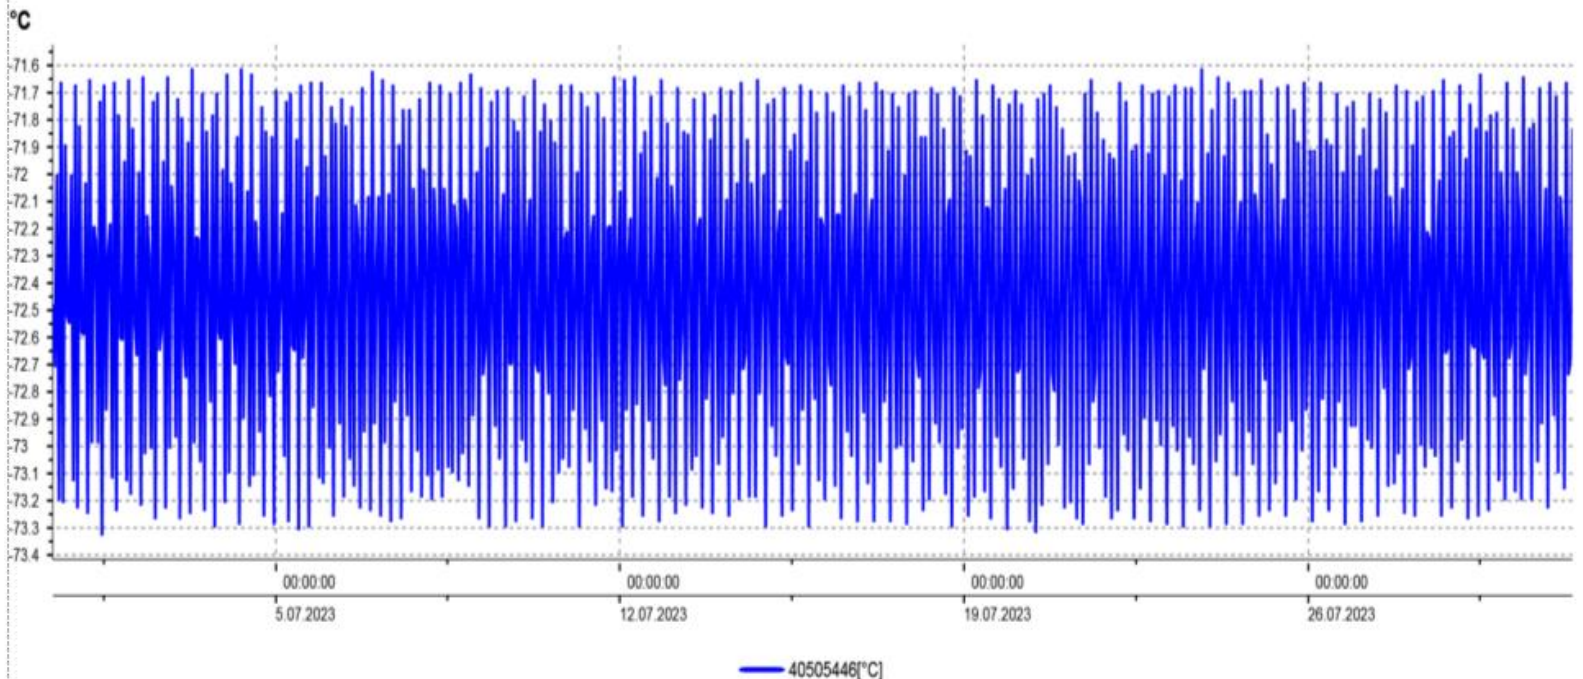

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31, Jul 2023 ~ 31, Aug 2023

Instrument name: Testo 176T2		2023/9/4 上午 09:35:41			Page 1/1
Start time: 2023/7/31 上午 09:22:28		Minimum	Maximum	Mean value	Limit values
End time: 2023/8/31 下午 03:22:28	40505446 [°C]	-82.20	-71.09	-73.632	-90.0/-60.0
Measurement channels: 1					
Measured values: 751					
SN 40505446					

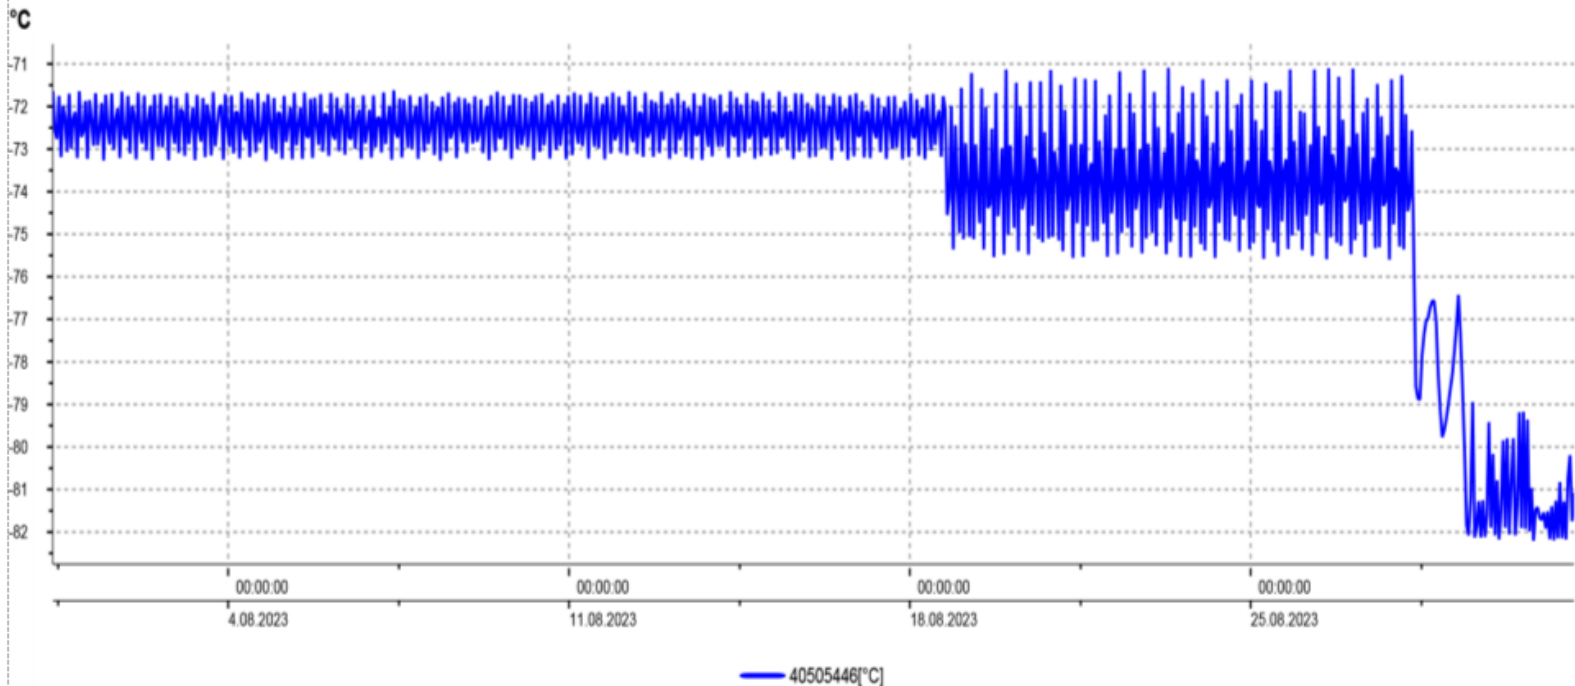

Comment: 2023/8/28~8/31設定溫度暫時調降。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 28, Sep 2023 ~ 31, Oct 2023

Instrument name: Testo 176T2		2023/11/2 下午 04:23:13			Page 1/1
Start time: 2023/9/28 下午 04:25:12		Minimum	Maximum	Mean value	Limit values
End time: 2023/10/31 上午 10:25:12	40505446 [°C]	-75.09	-72.84	-73.982	-80.0/-60.0
Measurement channels: 1					
Measured values: 787					
SN 40505446					

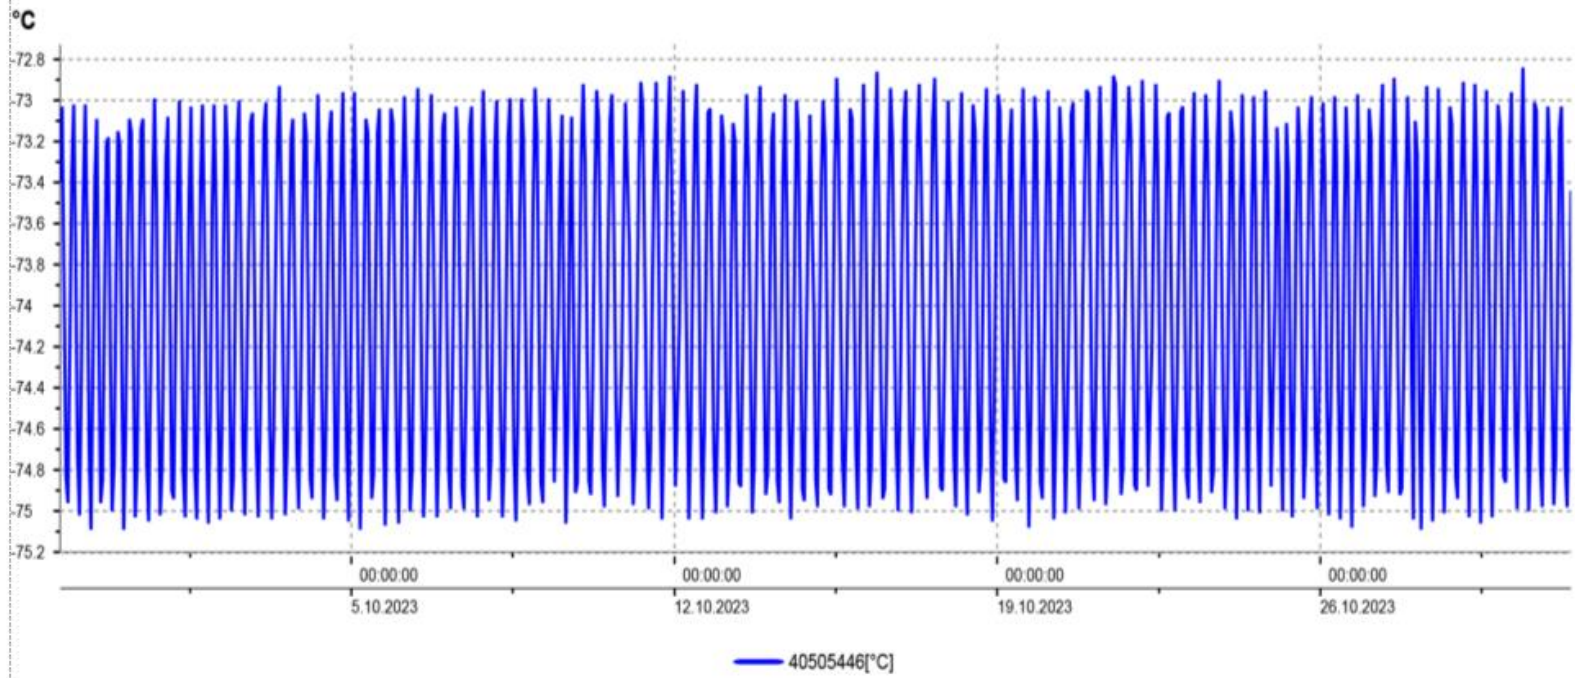

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31, Oct 2023 ~ 30, Nov 2023

Instrument name: Testo 176T2		2023/12/1 上午 10:50:13			Page	1/1
Starttime: 2023/10/31 上午 11:14:40		Minimum	Maximum	Mean value	Limit values	
End time: 2023/11/30 上午 10:14:40	40505446 [°C]	-75.13	-72.68	-73.907	-80.0/-80.0	
Measurement channels: 1						
Measured values: 720						
SN 40505446						

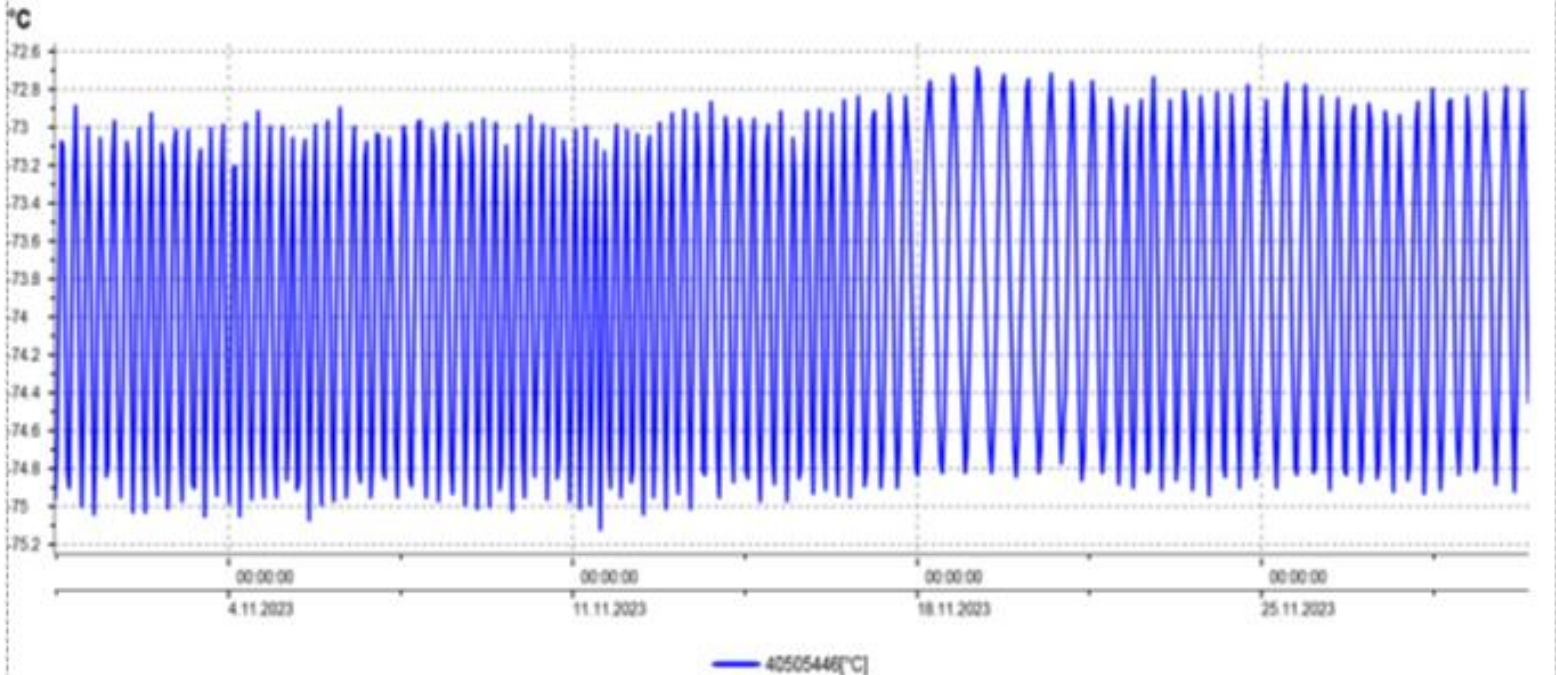

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 30, Nov 2023 ~ 29, Dec 2023

Instrument name: Testo 176T2		2023/12/29 下午 02:30:18			Page 1/1
Starttime: 2023/11/30 上午 11:00:29		Minimum	Maximum	Mean value	Limit values
Endtime: 2023/12/29 上午 10:00:29	40505446 [°C]	-74.97	-72.59	-73.812	-80.0/-80.0
Measurement channels: 1					
Measured values: 696					
SN 40505446					

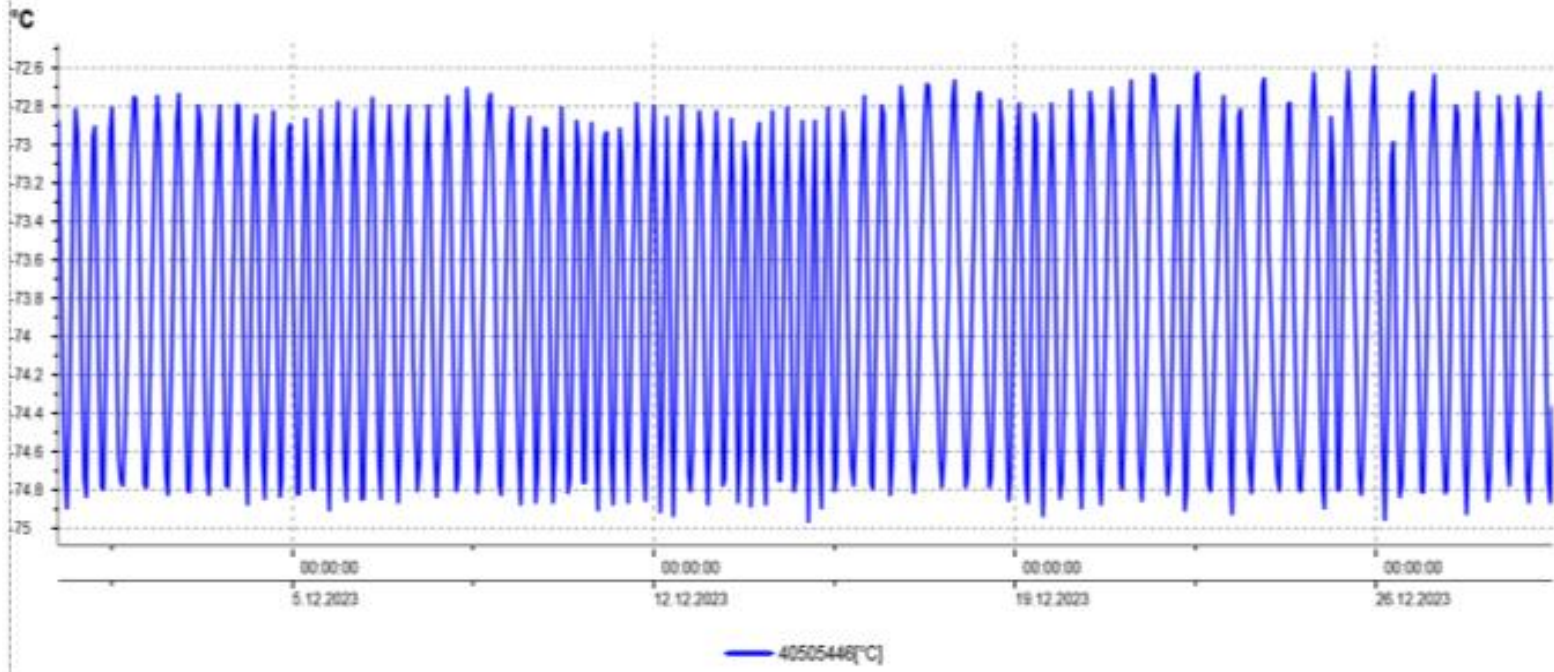

Comment: