

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 03, Jan 2023 ~ 30, Jan 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.4 -75.0 -79.95 0.88 -79.84

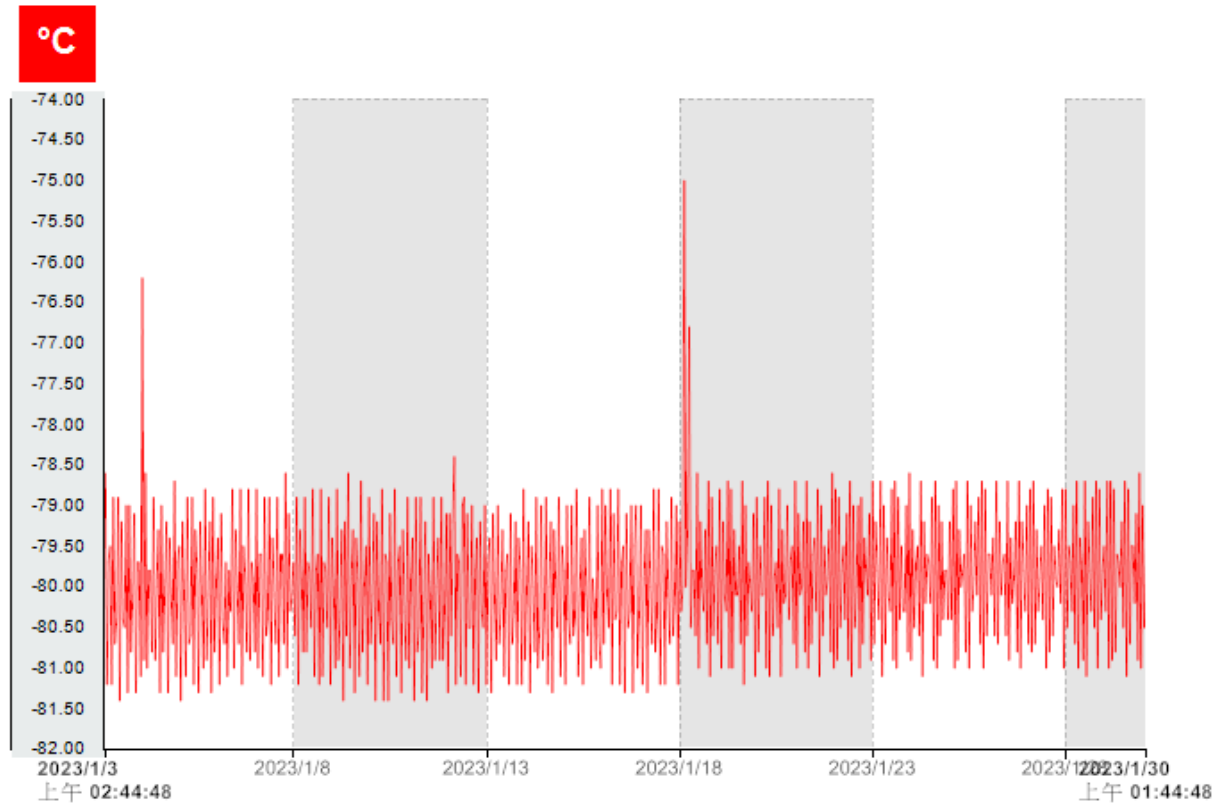

Comment: 因下載溫度用之筆電的時區有誤，此月份溫度記錄顯示之開始與結束時間比實際時間早8hr。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 30, Jan 2023 ~ 01, Mar 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.4 -74.5 -80.02 0.88 -79.91

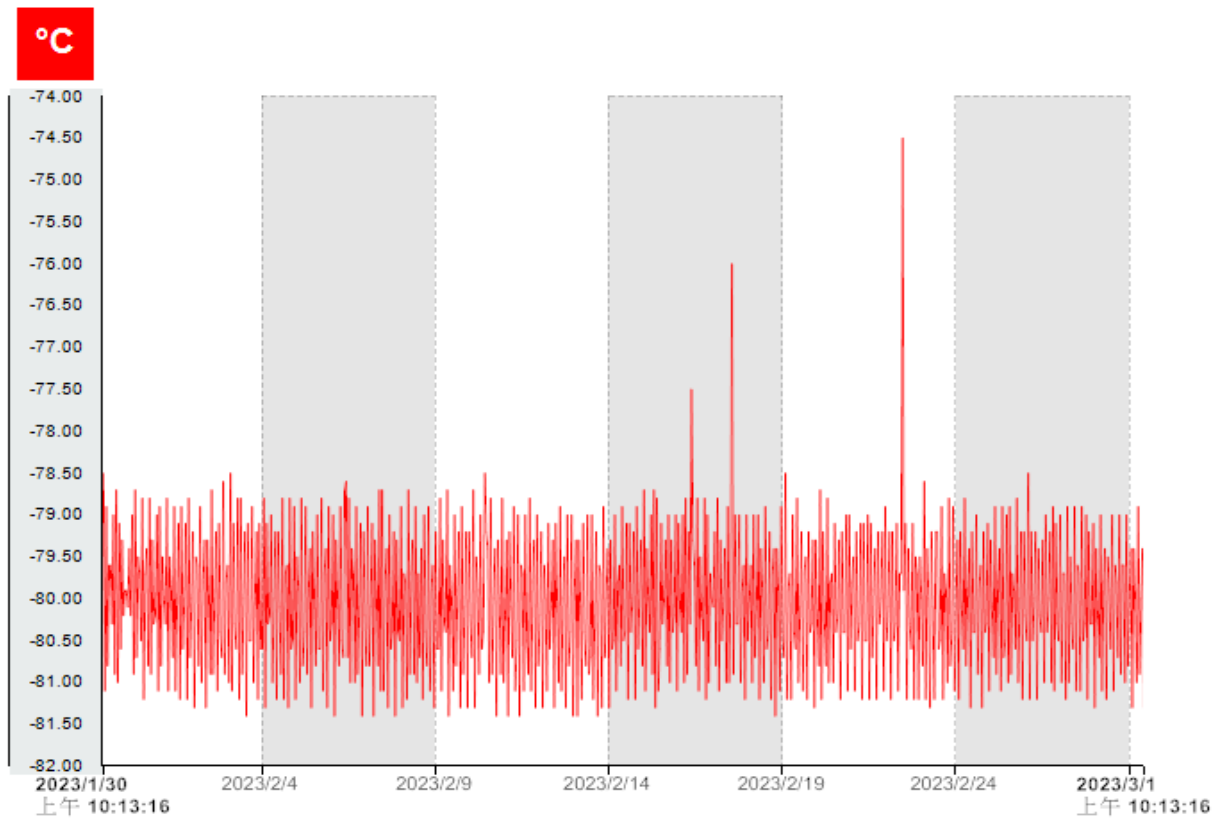

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 01, Mar 2023 ~ 31, Mar 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.4 -75.5 -80.03 0.84 -79.93

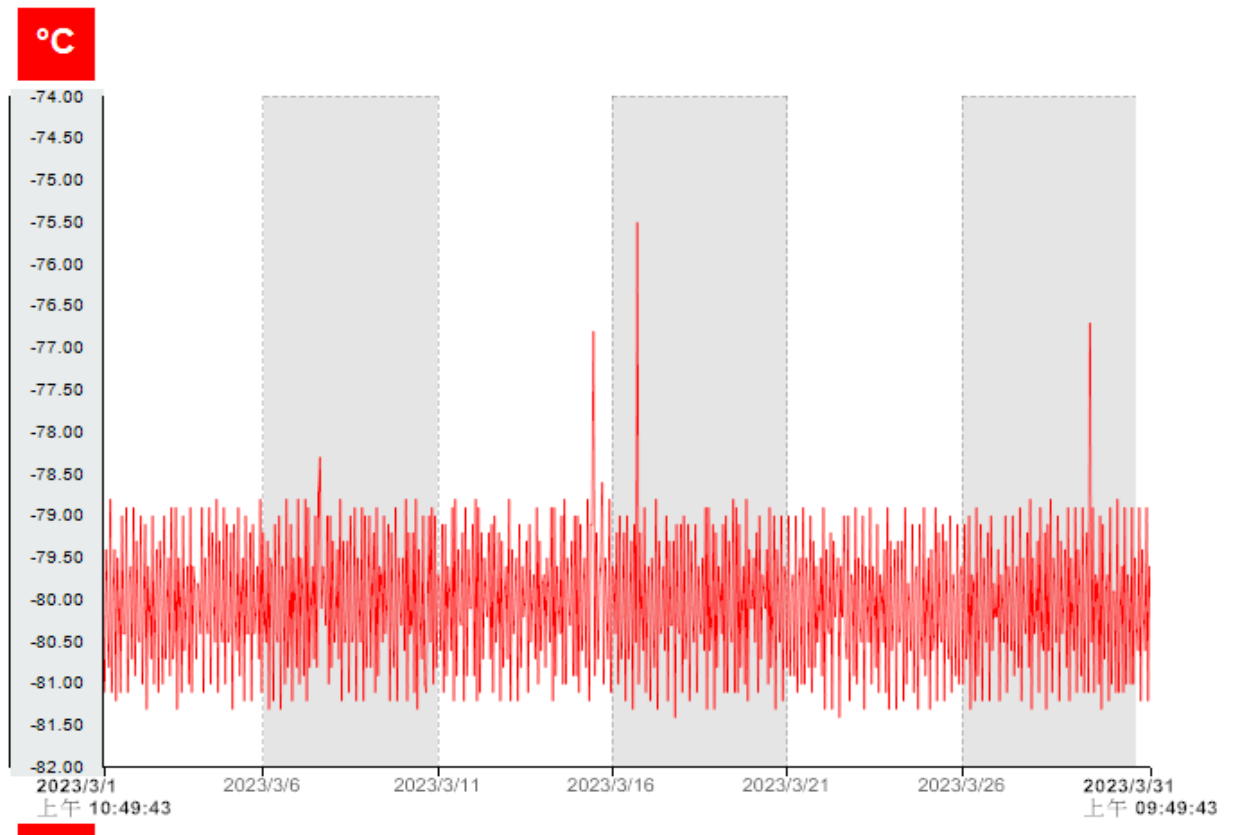

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 31, Mar 2023 ~ 28, Apr 2023



2K 190114208

v1 [°C]
Min Max Avg Sd MKT
-81.5 -77.1 -80.11 0.82 -80.02

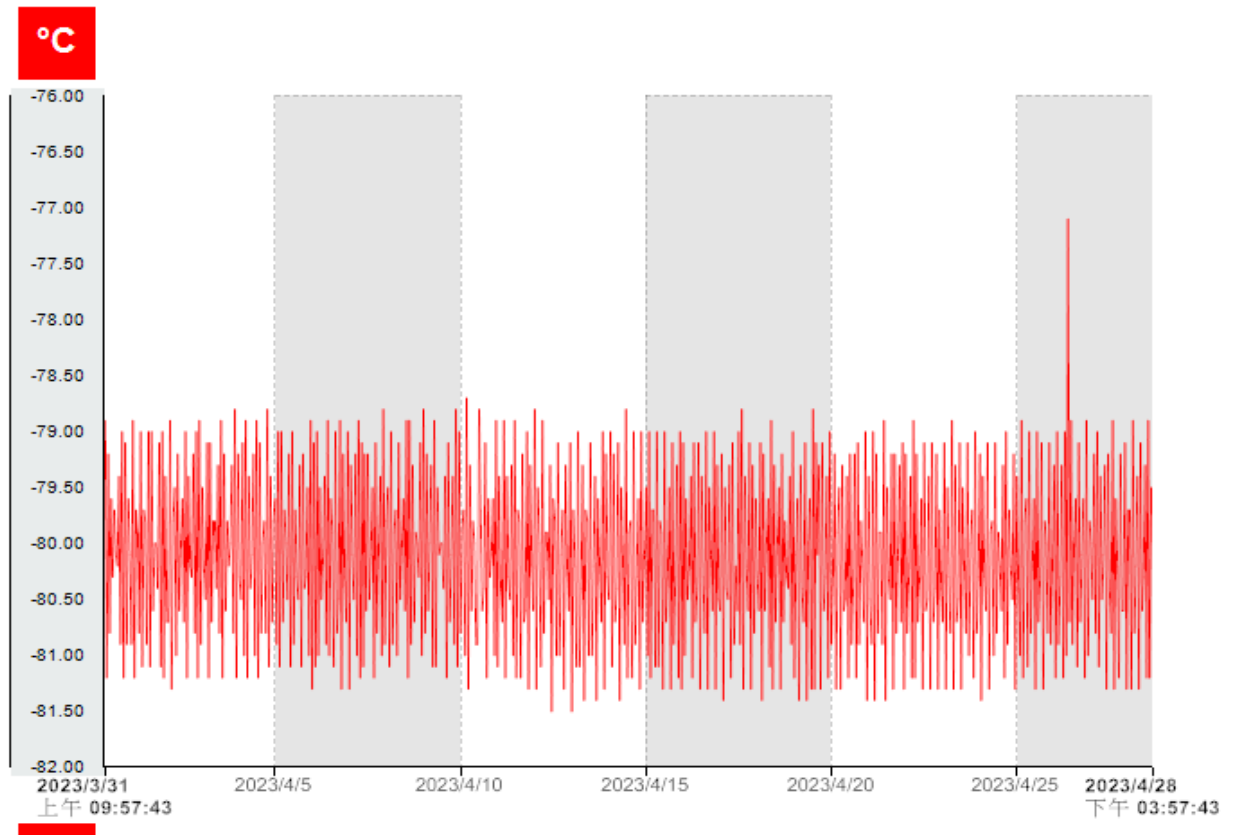

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 28, Apr 2023 ~ 29, May 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.6 -78.3 -80.16 0.84 -80.07

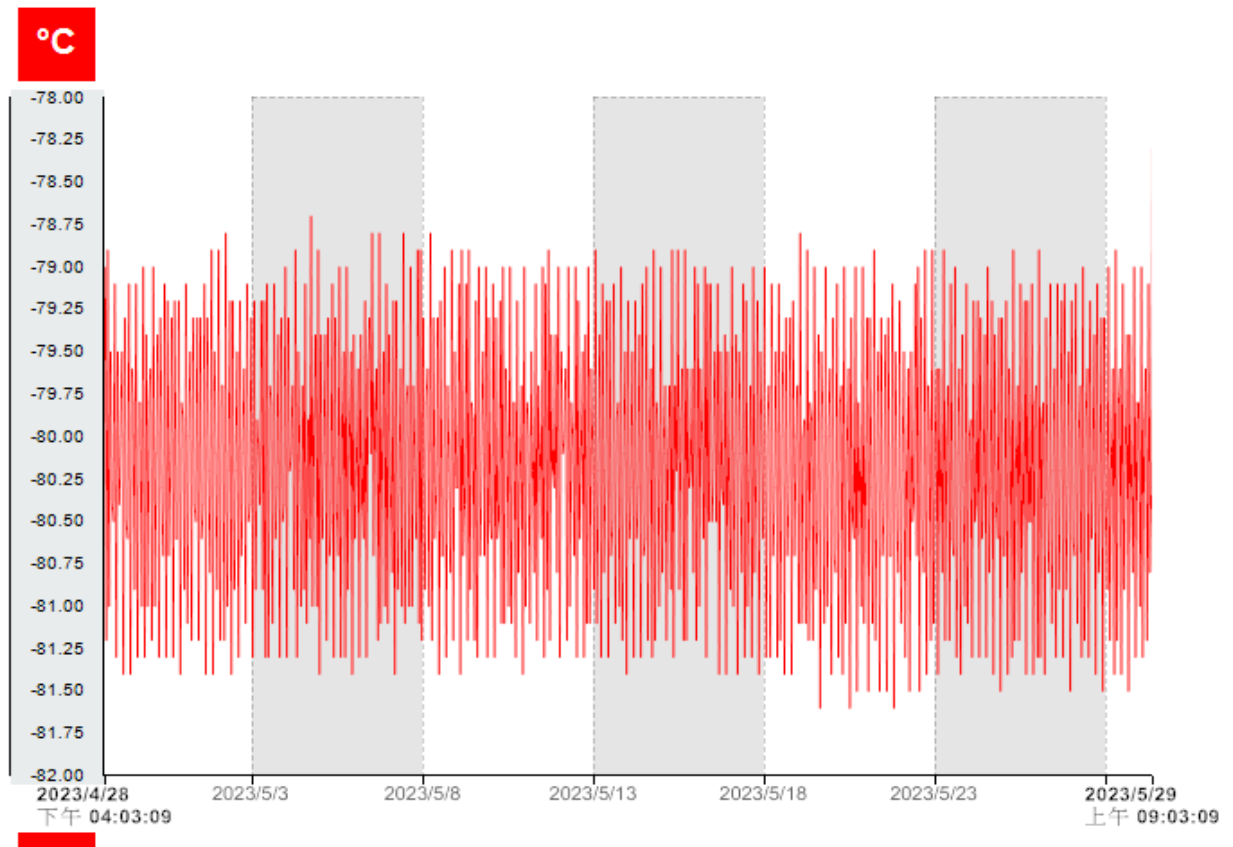

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 29, May 2023 ~ 30, Jun 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.6 -78.0 -80.23 0.83 -80.14

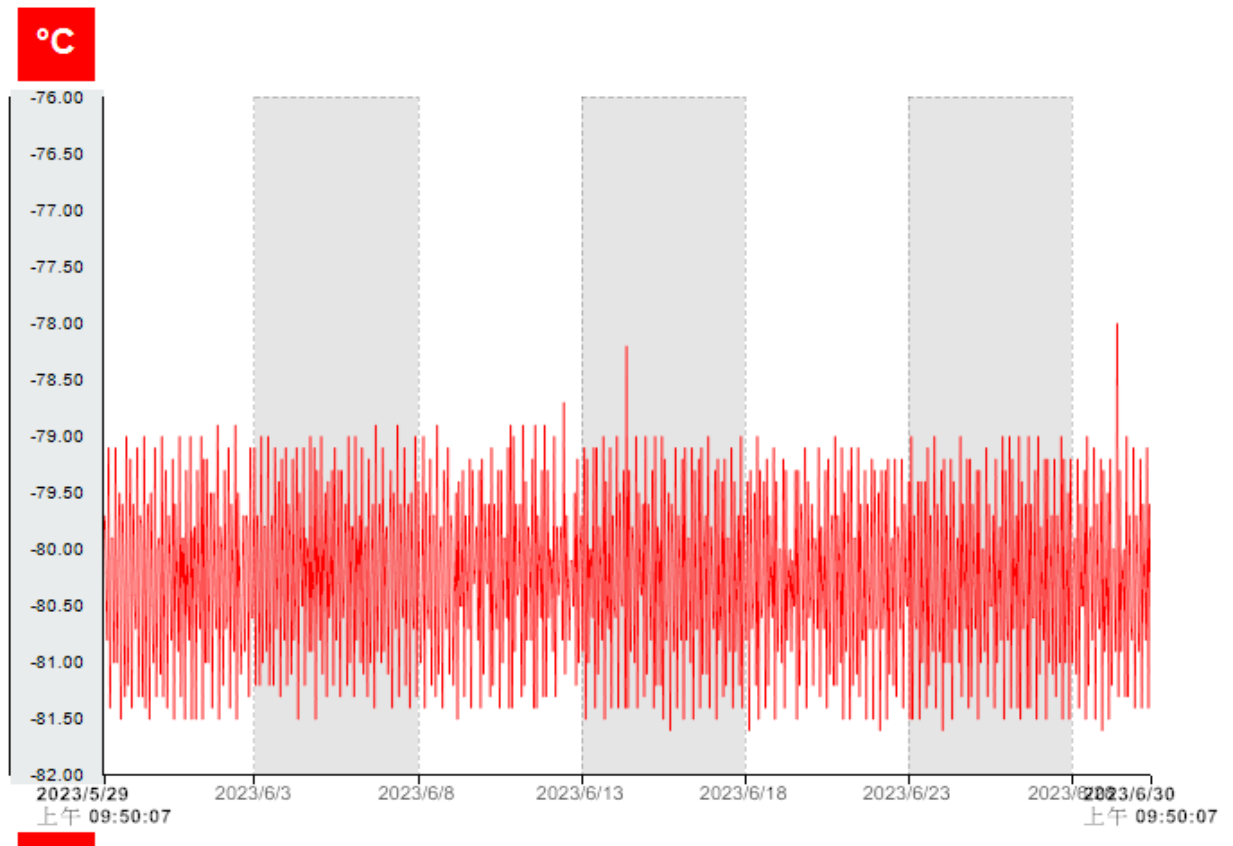

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-310; Serial No. : 12010863; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 30, Jun 2023 ~ 31, Jul 2023

KIMO 12010863

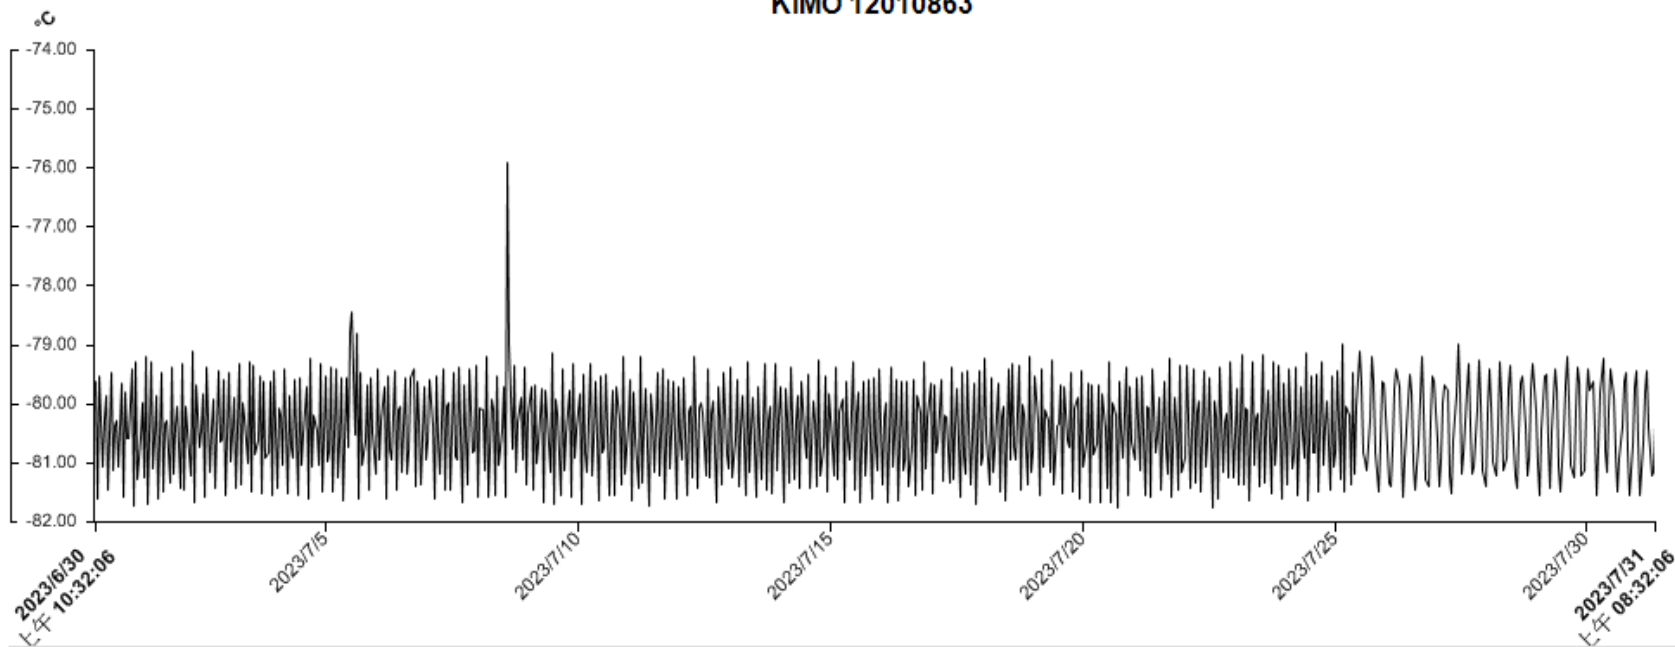

統計表

	#1
最小 T	-81.77
最小 t	-81.77
最大值 T	-75.91
最大值 t	-75.91
平均值 T	-80.418
平均值 t	-80.418
標準偏差 T	0.814
標準偏差 t	0.814
MKT T	-80.422
MKT t	-80.422

T: 整個週期
t: 顯示週期

Comment: 本溫度記錄器(2K190114208)於2023年6月30日送校，期間以備品溫度記錄器(12010863)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-310; Serial No. : 12010863; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 31, Jul 2023 ~ 01, Sep 2023

KIMO 12010863

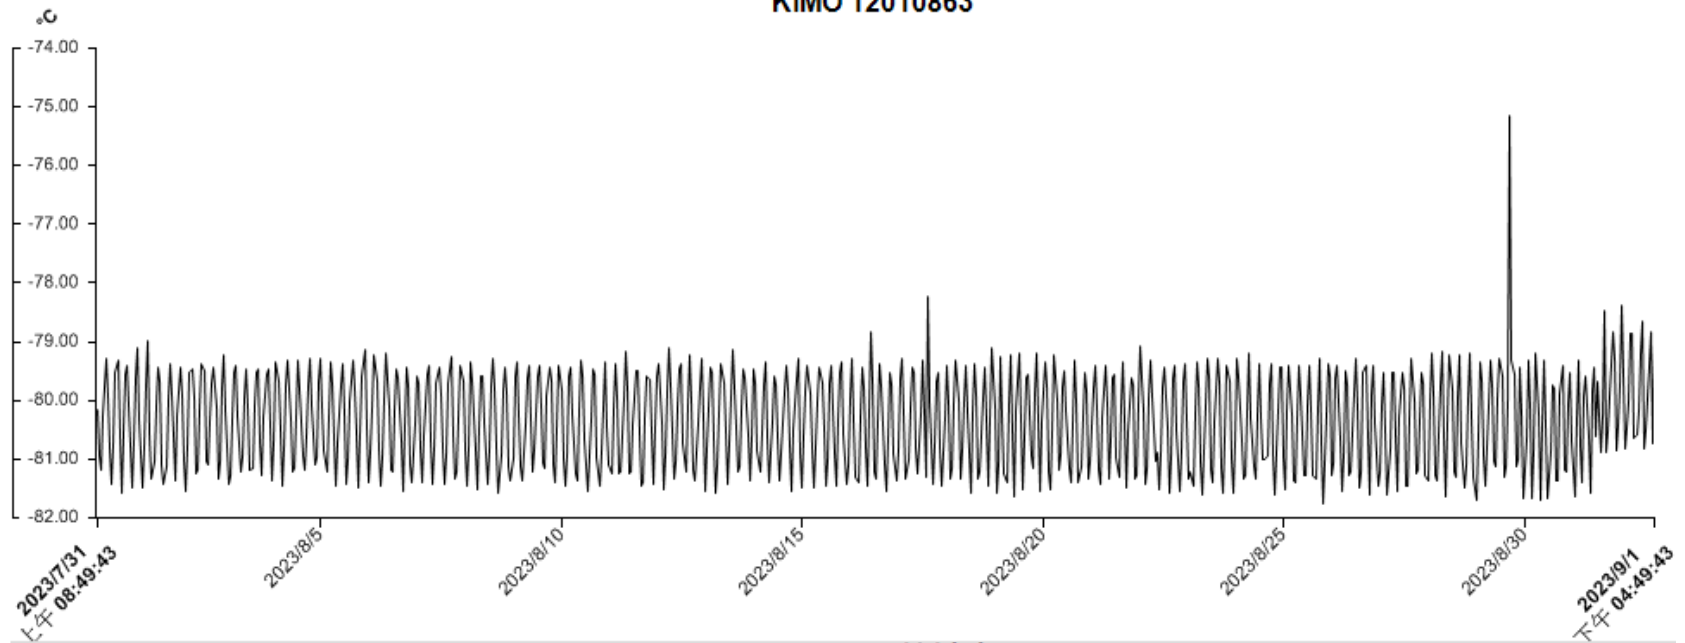

統計表

#1	
最小 T	-81.75
最小 t	-81.75
最大值 T	-75.14
最大值 t	-75.14
平均值 T	-80.35
平均值 t	-80.35
標準偏差 T	0.804
標準偏差 t	0.804
MKT T	-80.354
MKt t	-80.354

T: 整個週期
t: 顯示週期

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-310; Serial No. : 12010863; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80±10 °C

DATE : 01, Sep 2023 ~ 04, Sep 2023

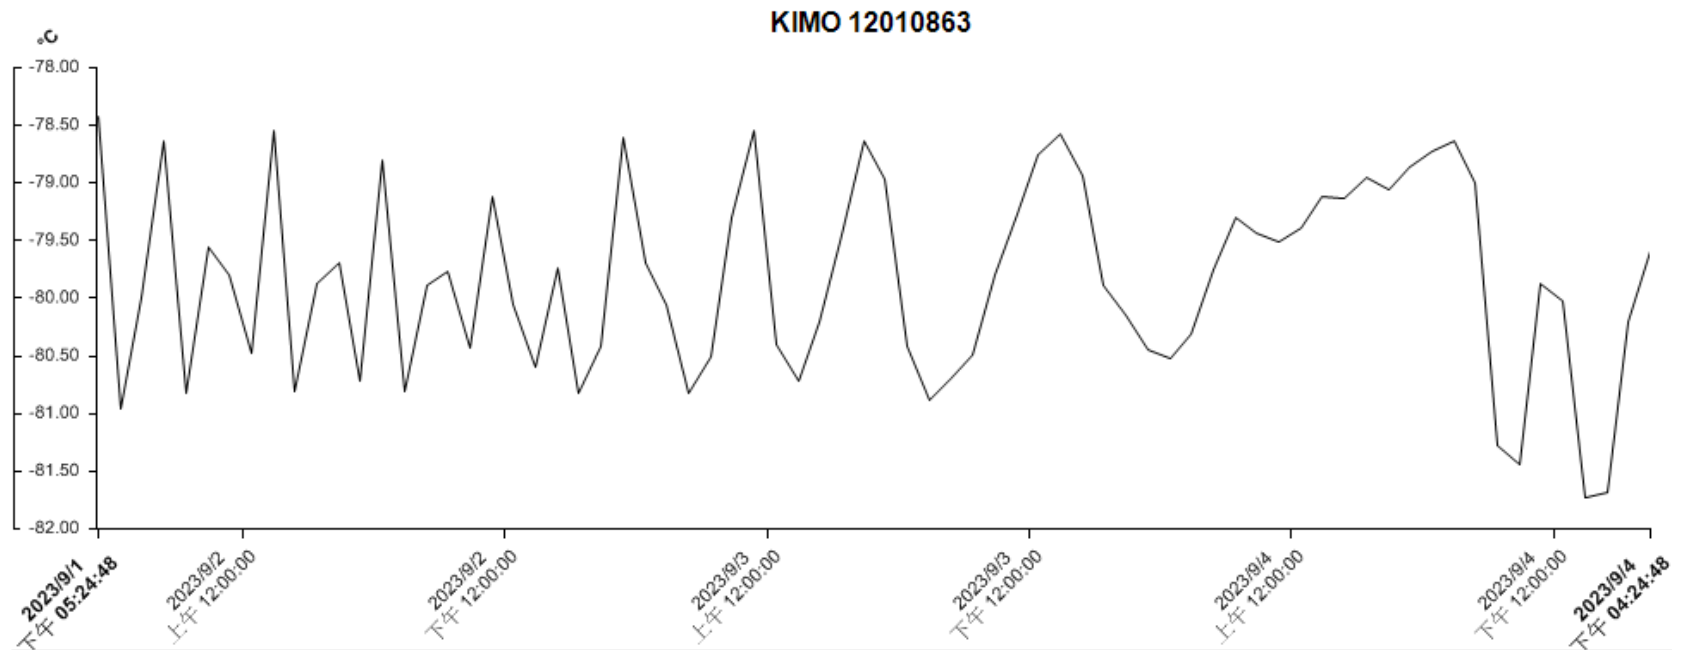

統計表

#1	
最小 T	-81.73
最小 t	-81.73
最大值 T	-78.42
最大值 t	-78.42
平均值 T	-79.84
平均值 t	-79.84
標準偏差 T	0.833
標準偏差 t	0.833
MKT T	-79.843
MKT t	-79.843

T: 整個週期
t: 顯示週期

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80 ± 10 °C

DATE : 04, Sep 2023 ~ 28, Sep 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-82.1 -79.0 -80.71 0.84 -80.62

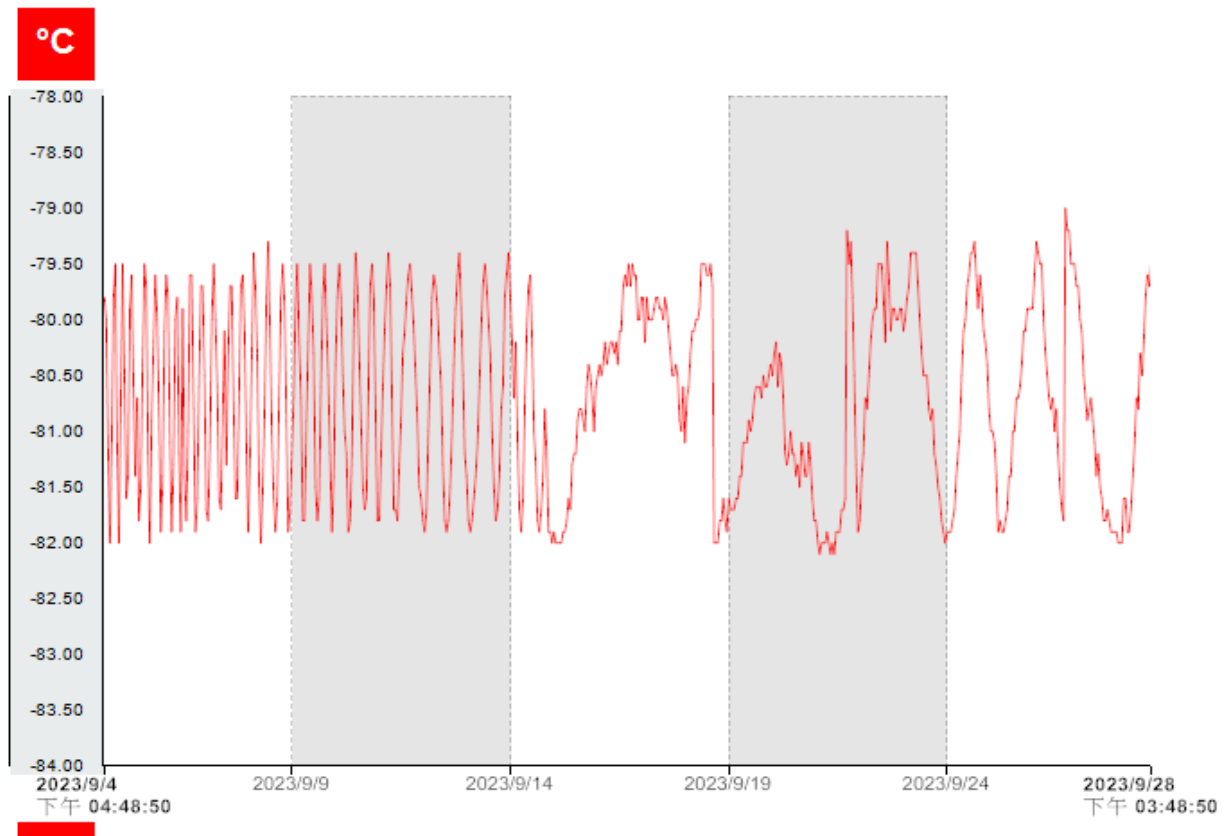

Comment: 本溫度記錄器(2K190114208)完成校正，於2023年9月4日換回使用。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 28, Sep 2023 ~ 31, Oct 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-82.0 -75.5 -80.61 0.83 -80.51

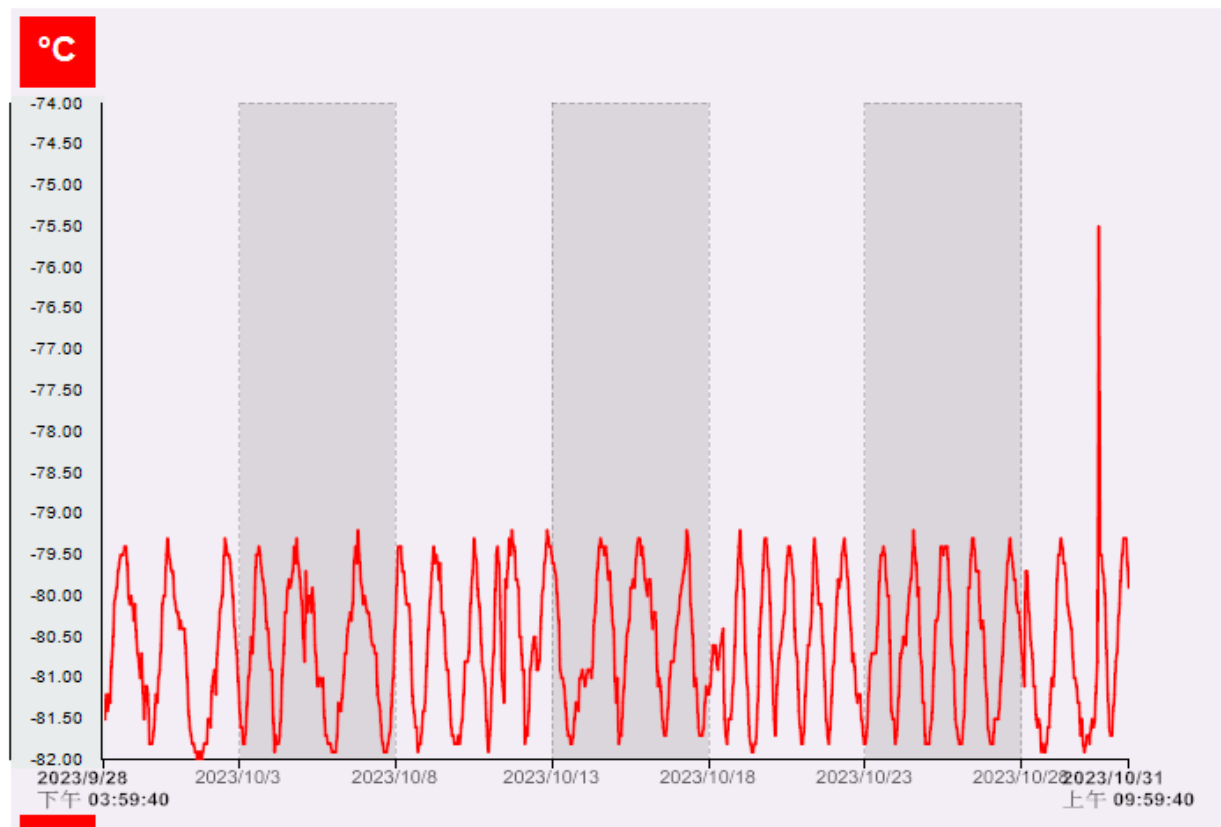

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 31, Oct 2023 ~ 30, Nov 2023



2K 190114208

— v1 [°C]

Min	Max	Avg	Sd	MKT
-82.0	-79.2	-80.56	0.85	-80.46



Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer : PHCbi ; Model No. : MPF-DU302VX-PA; Serial No. : 19070046

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O ; Serial No. : 2K190114208; Channel No. : 1


REFRIGERATOR TEMPERATURE RANGE : -80± 10 °C

DATE : 30, Nov 2023 ~ 29, Dec 2023



2K 190114208

— v1 [°C]
Min Max Avg Sd MKT
-81.9 -79.0 -80.47 0.81 -80.38

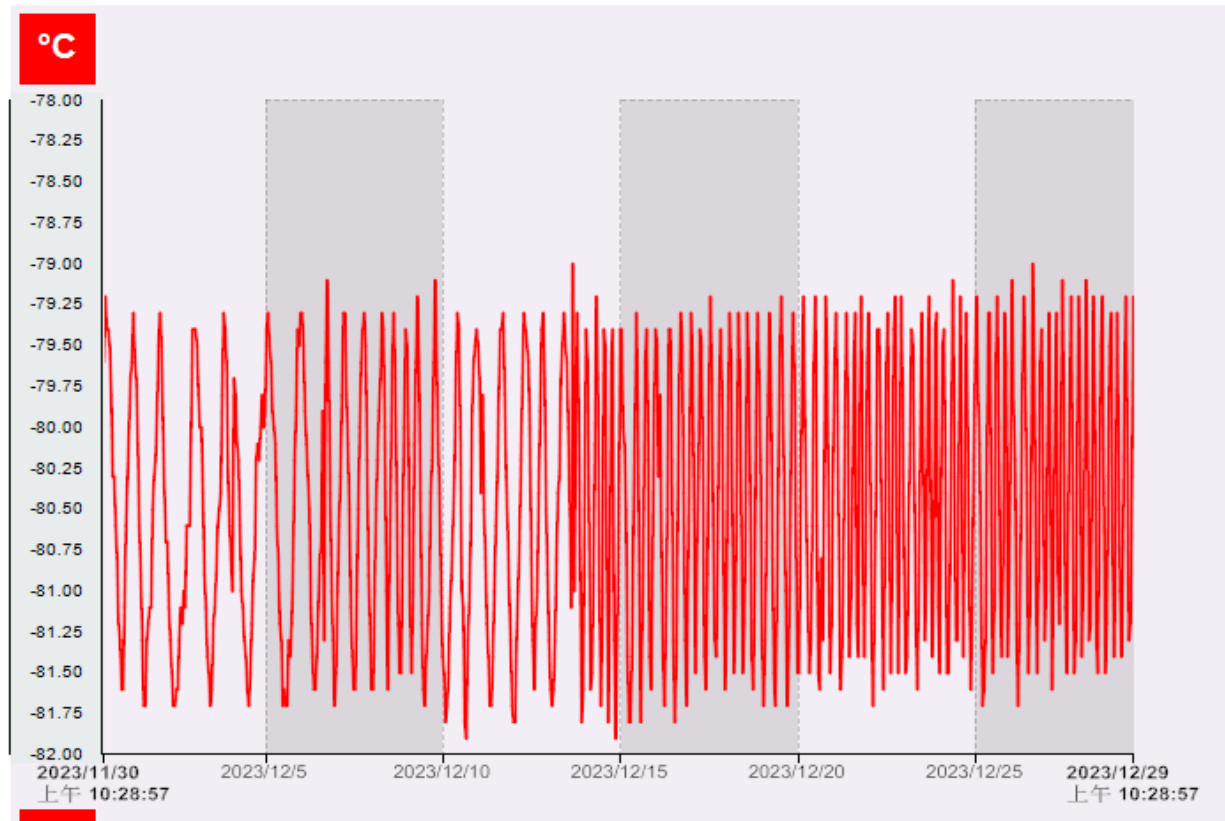

Comment: