

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : KIMO; Model No. : KTT-310; Serial No.: 1305 1667; Channel No.: 1

FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 03, Jan 2023 ~ 30, Jan 2023

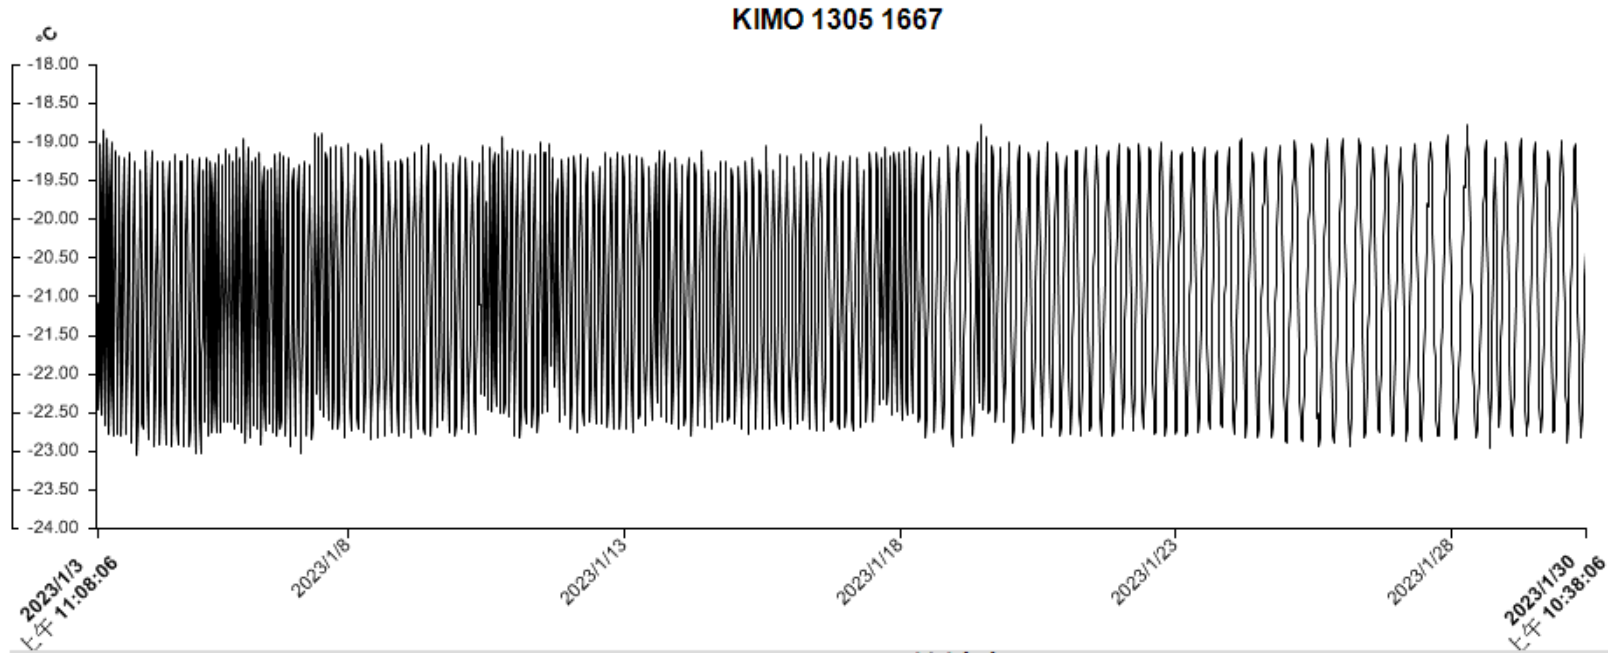

統計表

	#1
最小 T	-23.04
最小 t	-23.04
最大值 T	-18.77
最大值 t	-18.77
平均值 T	-20.965
平均值 t	-20.965
標準偏差 T	1.254
標準偏差 t	1.254
MKT T	-20.971
MKT t	-20.971

T: 整個週期
t: 顯示週期

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : KIMO; Model No. : KTT-310; Serial No.: 1305 1667; Channel No.: 1

FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Jan 2023 ~ 01, Mar 2023

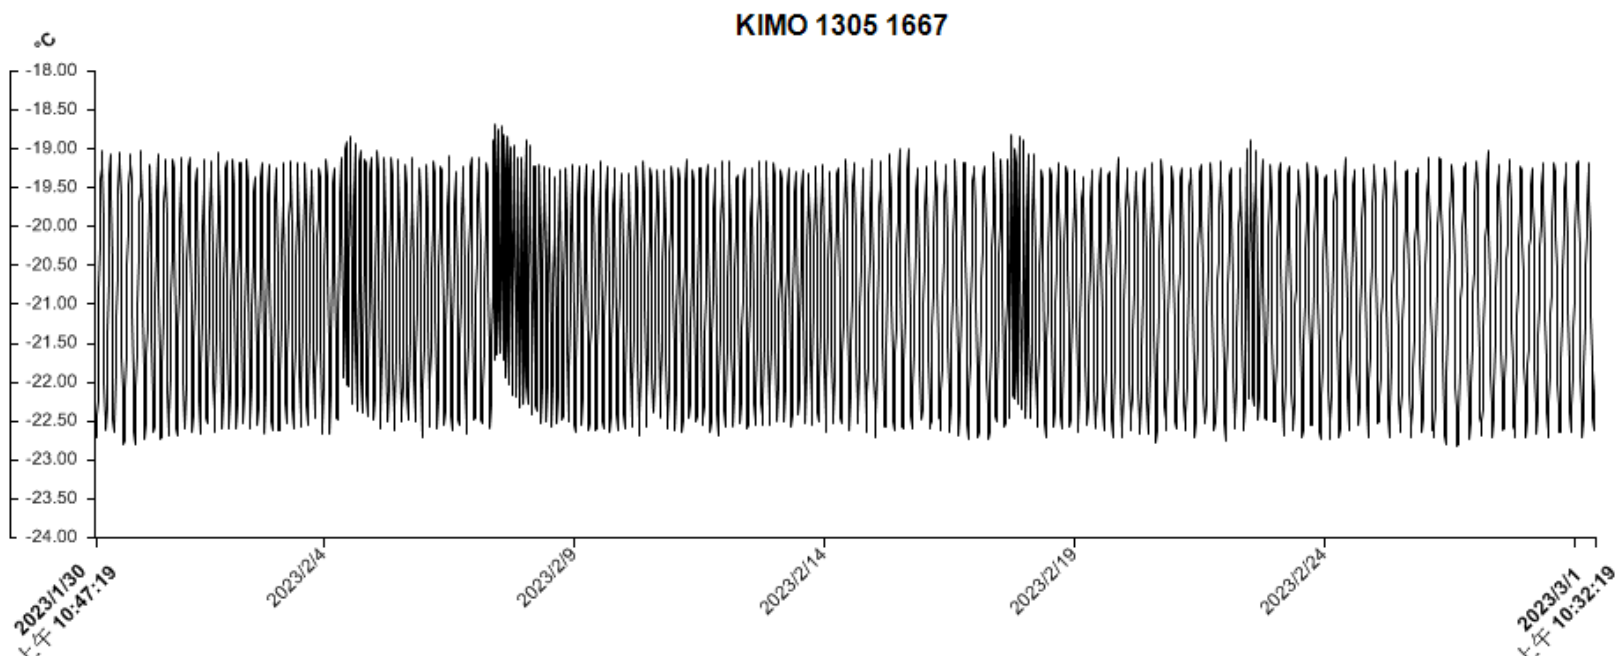

統計表

	#1
最小 T	-22.82
最小 t	-22.82
最大值 T	-18.69
最大值 t	-18.69
平均值 T	-20.905
平均值 t	-20.905
標準偏差 T	1.179
標準偏差 t	1.179
MKT T	-20.911
MKT t	-20.911

T: 整個週期
t: 顯示週期

Comment: 因冷凍2下層除霜，本冷凍櫃（冷凍1）於2023年2月17日08:50開始儲存藥品，並於2023年2月20日09:00將藥品移回冷凍2下層。

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : KIMO; Model No. : KTT-310; Serial No.: 1305 1667; Channel No.: 1

FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 01, Mar 2023 ~ 25, Mar 2023

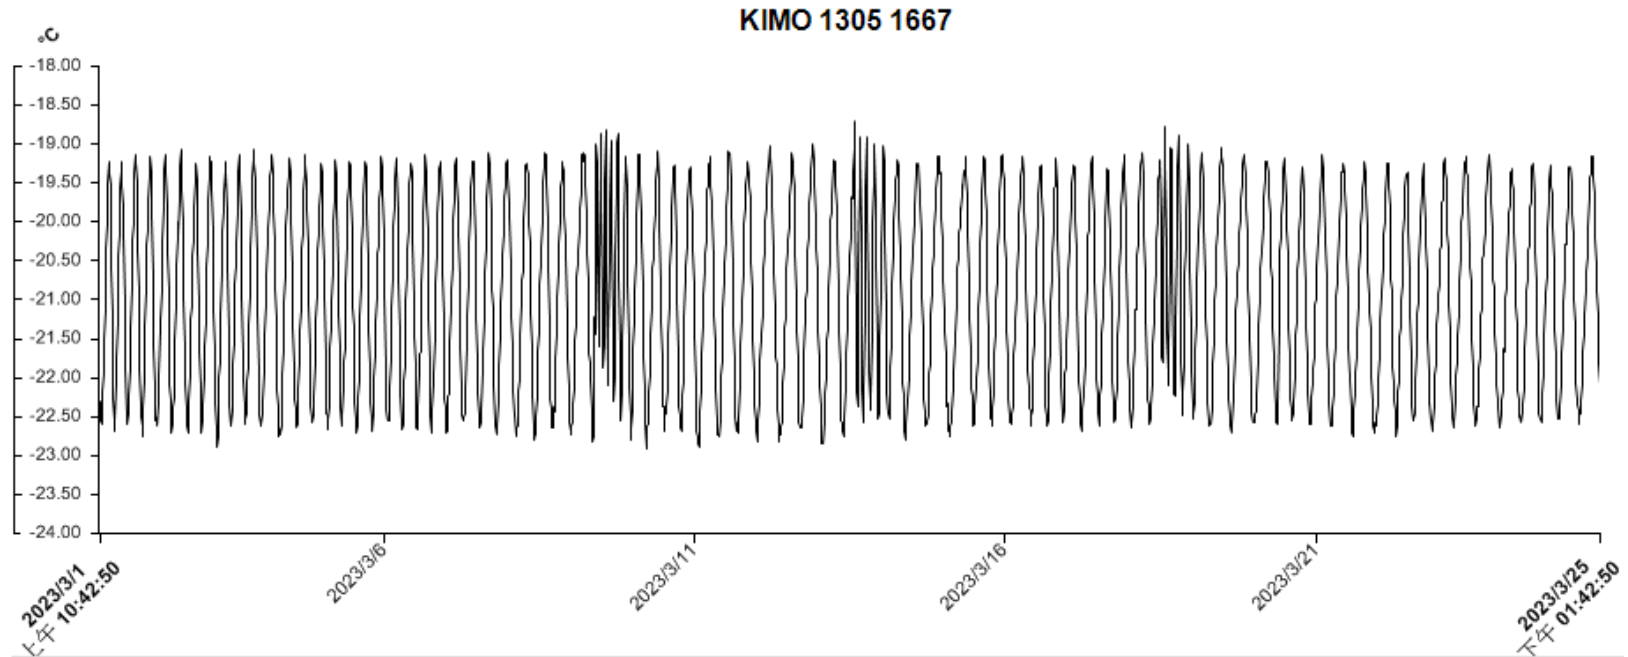

統計表

#1	
最小 T	-22.91
最小 t	-22.91
最大值 T	-18.71
最大值 t	-18.71
平均值 T	-20.926
平均值 t	-20.926
標準偏差 T	1.187
標準偏差 t	1.187
MKT T	-20.932
MKT t	-20.932

T: 整個週期
t: 顯示週期

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 27, Mar 2023 ~ 31, Mar 2023



KIMO 2K160903197

— v1 2K160903197 [°C]
Min Max Avg Sd MKT
-22.6 -18.8 -20.81 1.17 -20.71

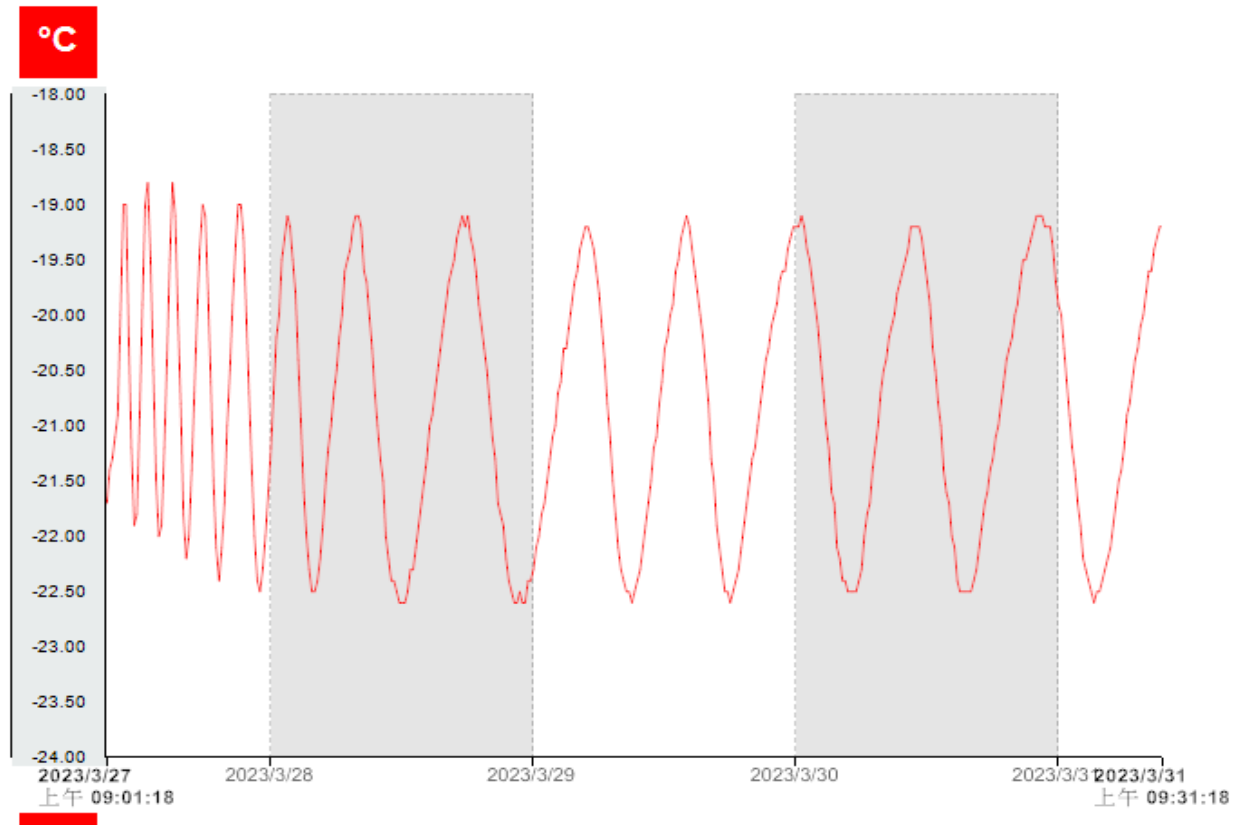

Comment: 原溫度記錄器(13051667)故障，2023/3/25 13:42至2023/3/27 09:01期間無溫度記錄，送修。期間以備品溫度記錄器(2K160903197)暫代。本冷藏櫃目前無存放藥品。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Mar 2023 ~ 28, Apr 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-22.7 -18.9 -20.86 1.15 -20.76

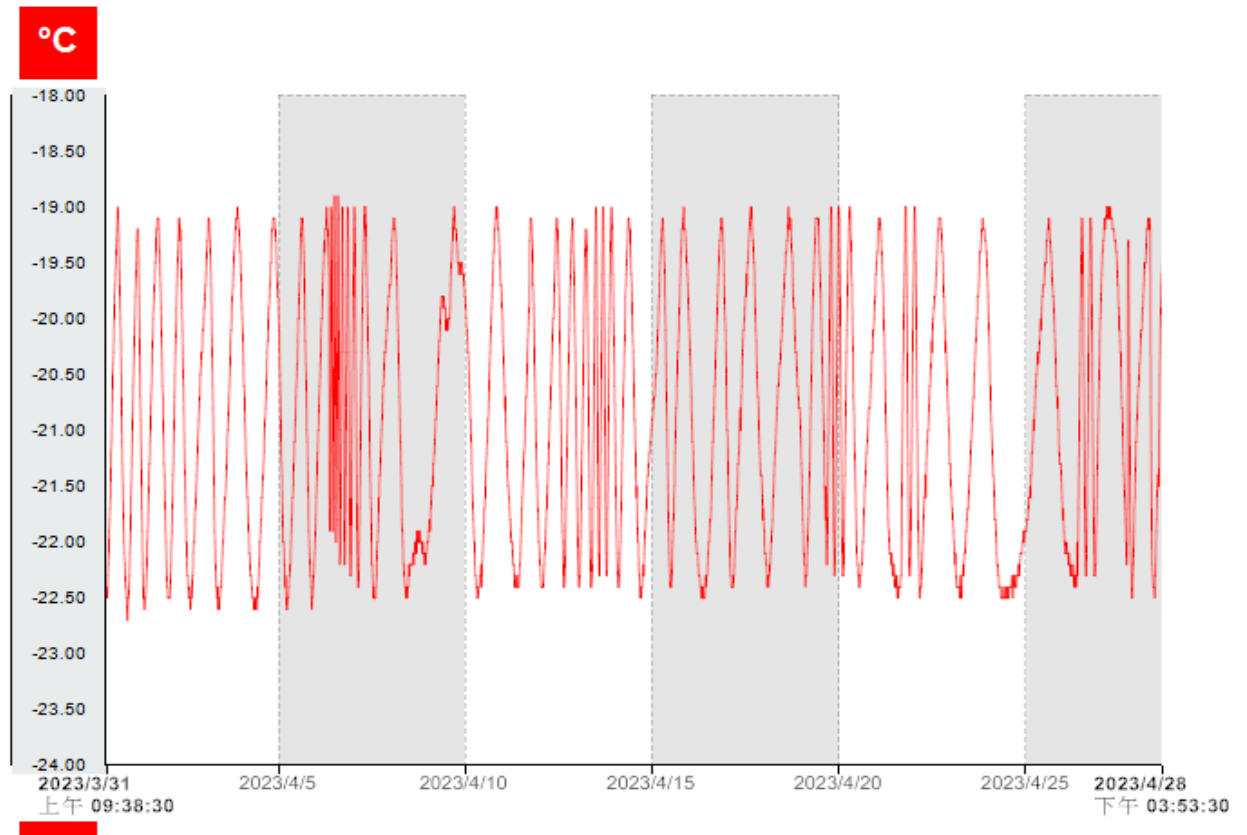

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 28, Apr 2023 ~ 29, May 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-22.6 -19.0 -20.87 1.07 -20.78

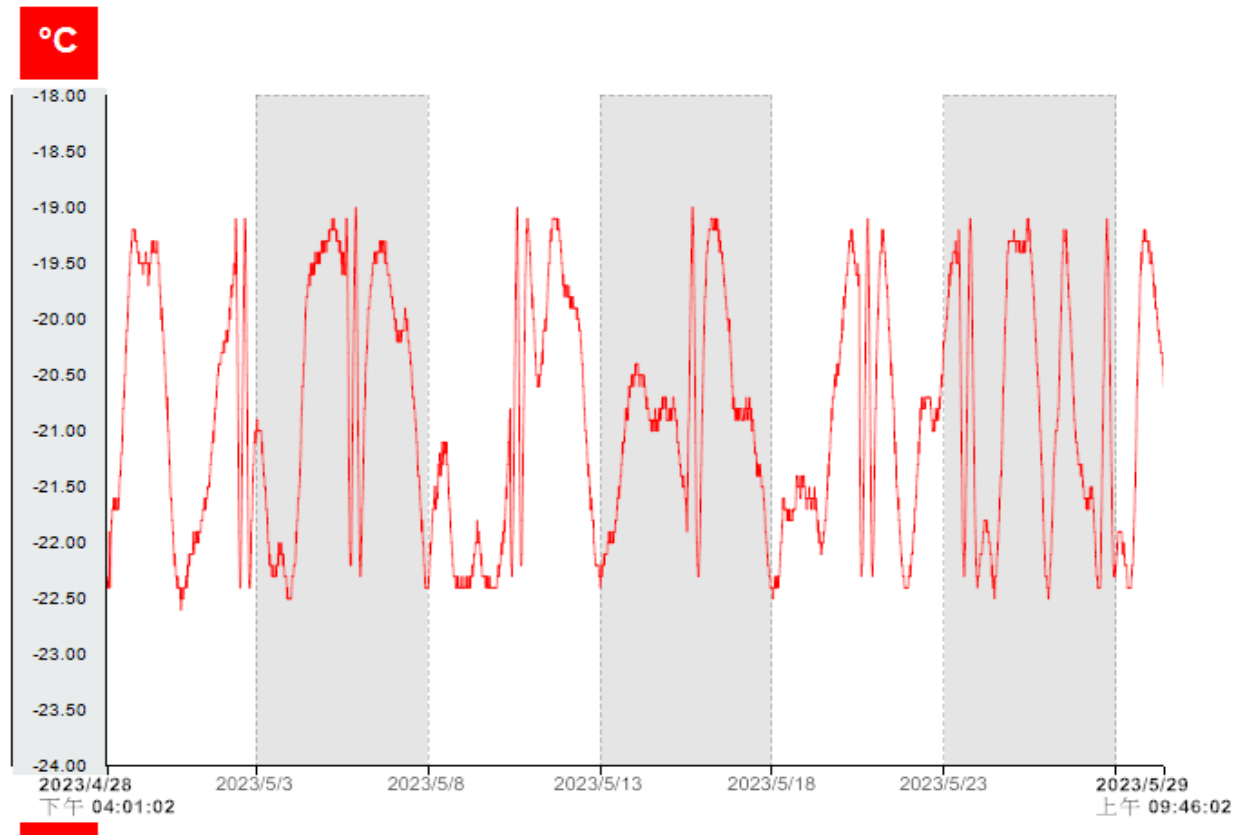

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 29, May 2023 ~ 30, Jun 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-22.5 -18.2 -20.80 1.08 -20.71

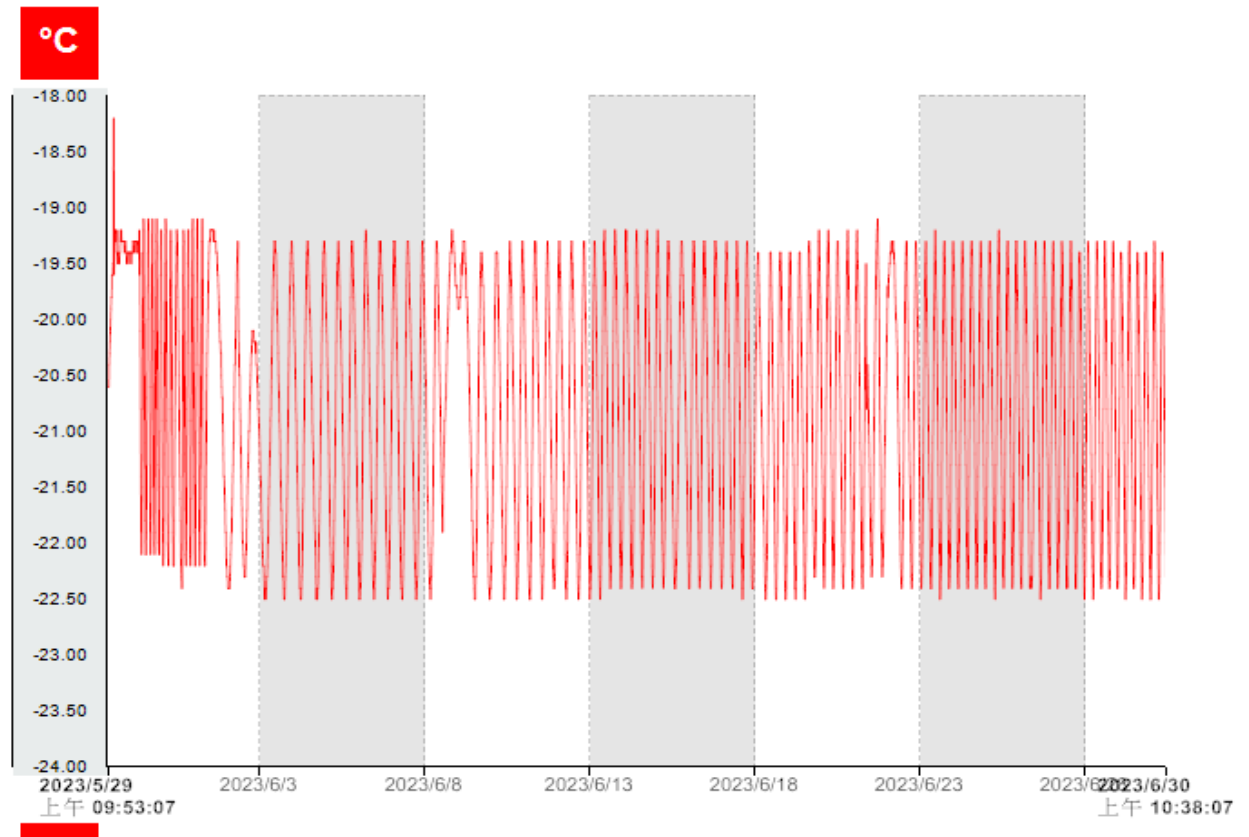

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Jun 2023 ~ 31, Jul 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-22.8 -16.9 -21.08 1.05 -21.00

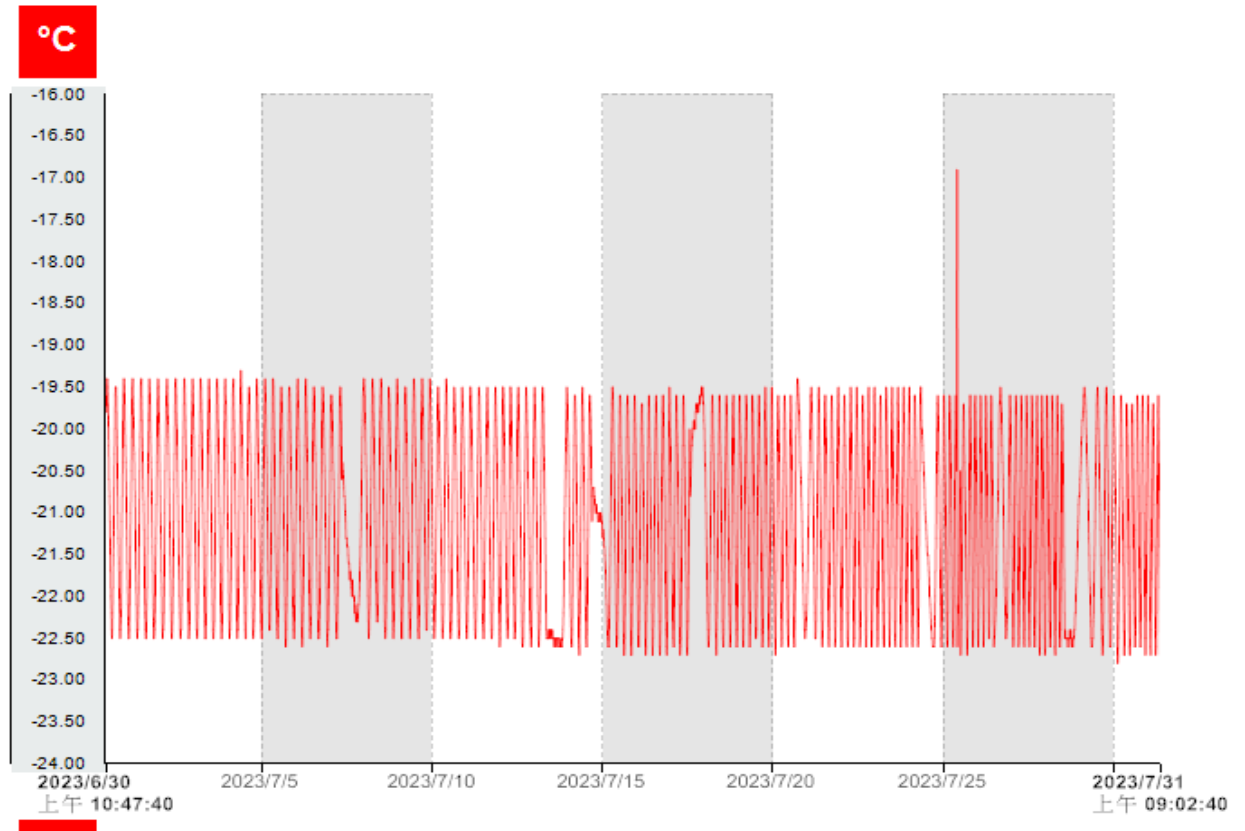

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Jul 2023 ~ 31, Aug 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-22.9 -19.3 -21.23 1.04 -21.15

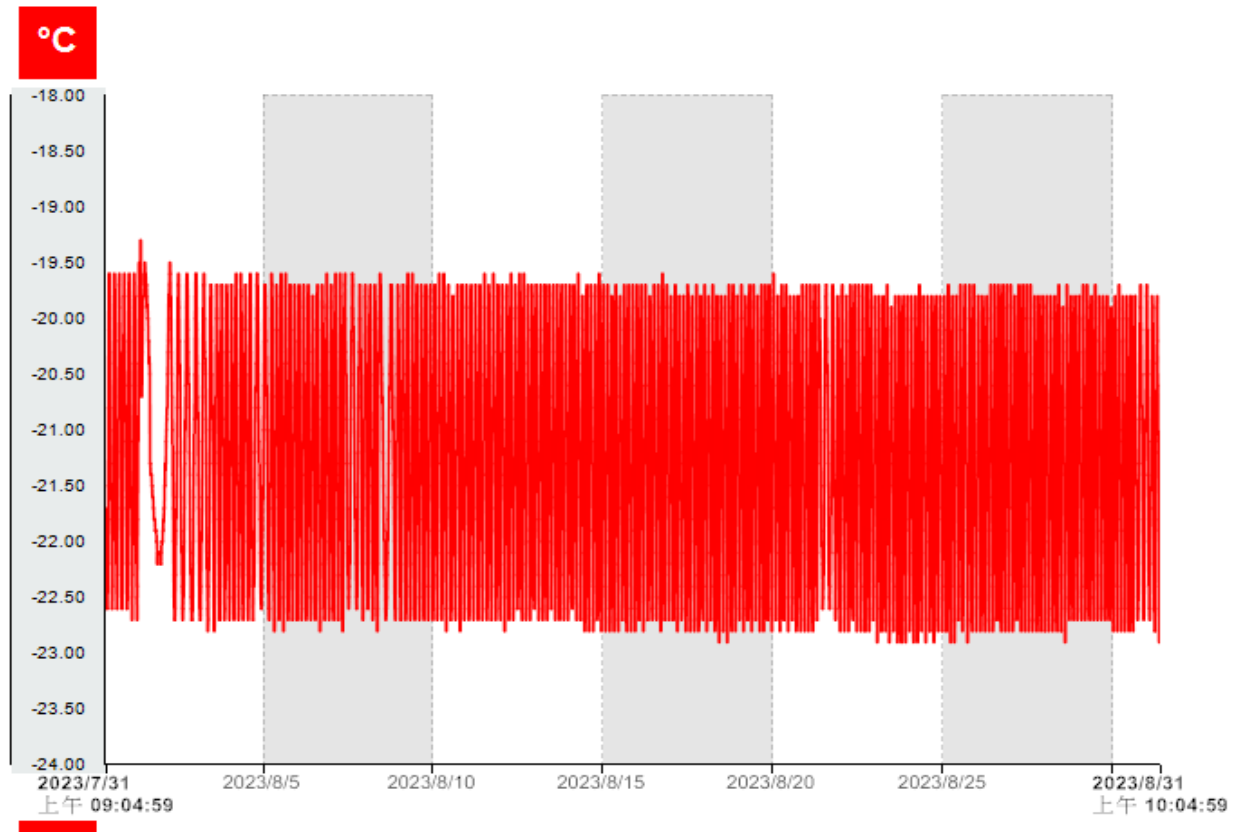

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Aug 2023 ~ 28, Sep 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-23.2 -18.0 -21.33 1.07 -21.25

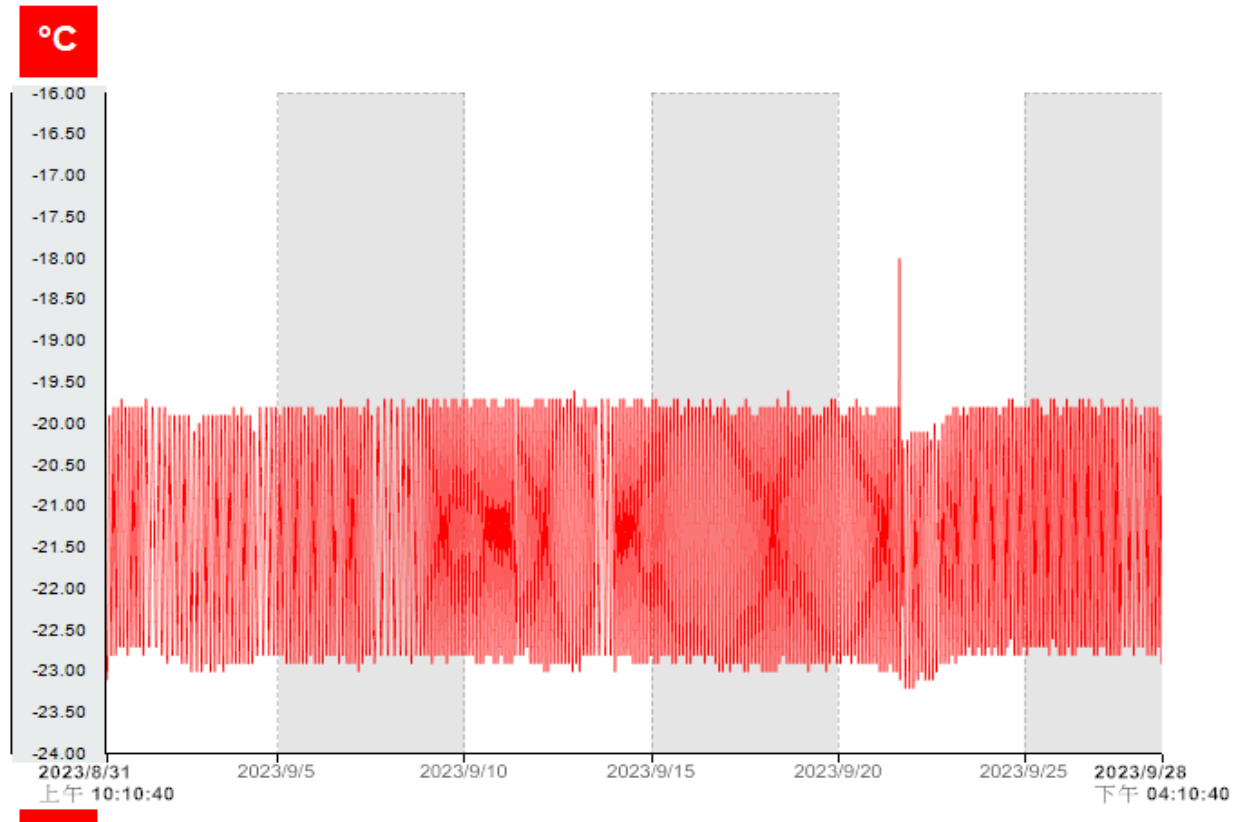

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 28, Sep 2023 ~ 31, Oct 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-23.1 -19.7 -21.37 1.05 -21.29

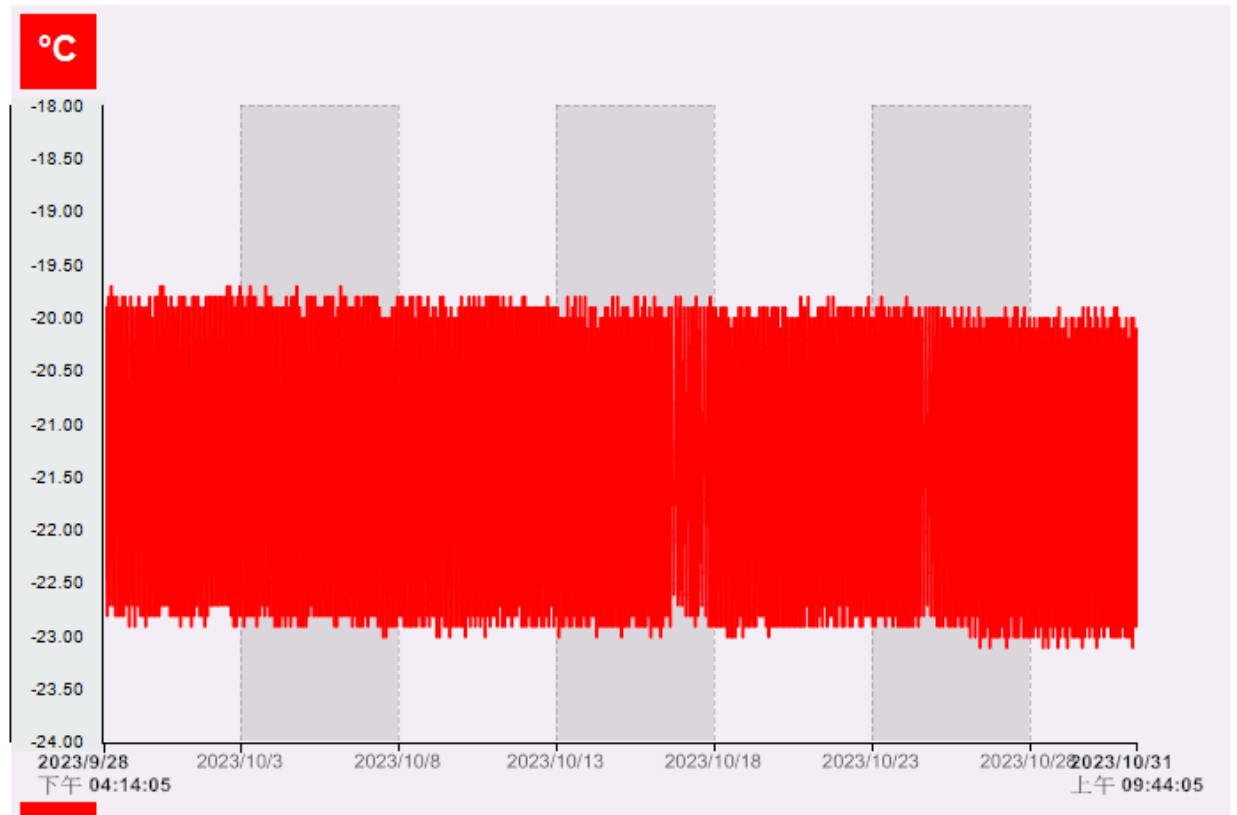

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1

FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Oct 2023 ~ 30, Nov 2023



KIMO 2K160903197

— v1 [°C]
Min Max Avg Sd MKT
-23.2 -19.8 -21.47 1.05 -21.39



Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

FREEZER : Manufacturer; PANASONIC; Model No.: MDF-U334-PT; Serial No.: 1308 0310

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K160903197; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Nov 2023 ~ 29, Dec 2023



KIMO 2K160903197

v1 [°C]				
Min	Max	Avg	Sd	MKT
-23.2	-19.8	-21.52	1.07	-21.44

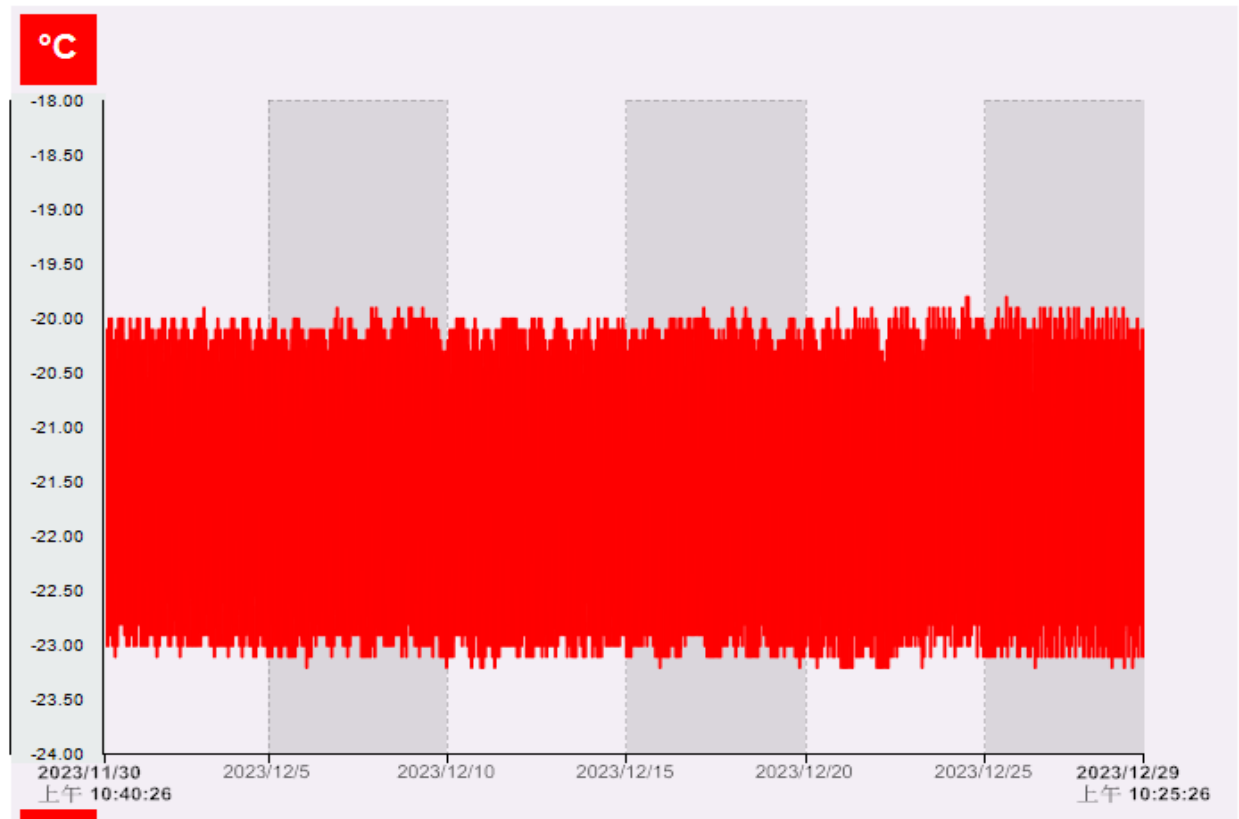

Comment: