

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 03, Jan 2023 ~ 30, Jan 2023



2K210923833

— v1 [°C]
Min Max Avg Sd MKT
-23.2 -18.8 -19.99 0.92 -19.93

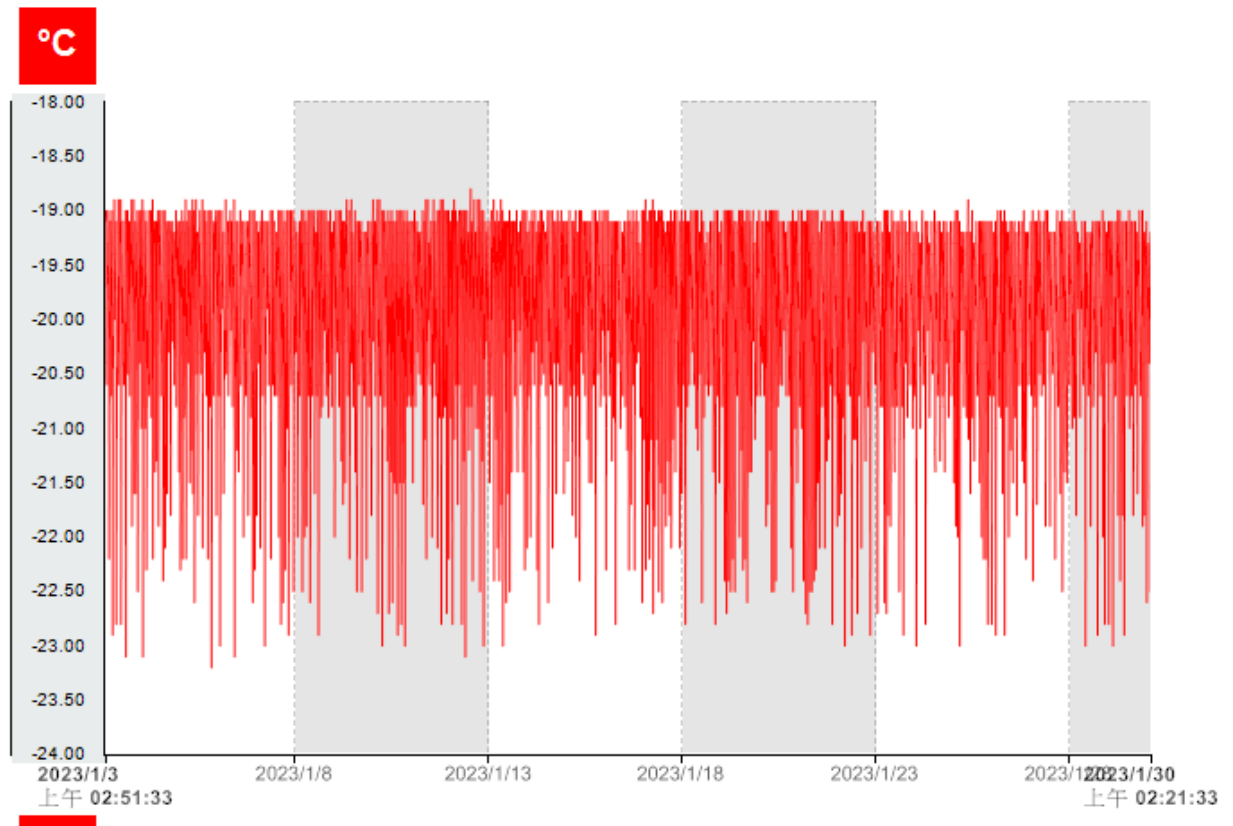

Comment: 因下載溫度用之筆電的時區有誤，此月份溫度記錄顯示之開始與結束時間比實際時間早8hr。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Jan 2023 ~ 01, Mar 2023



2K210923833

—	v1 [°C]				
Min	Max	Avg	Sd	MKT	
-23.8	-14.3	-19.99	0.97	-19.92	

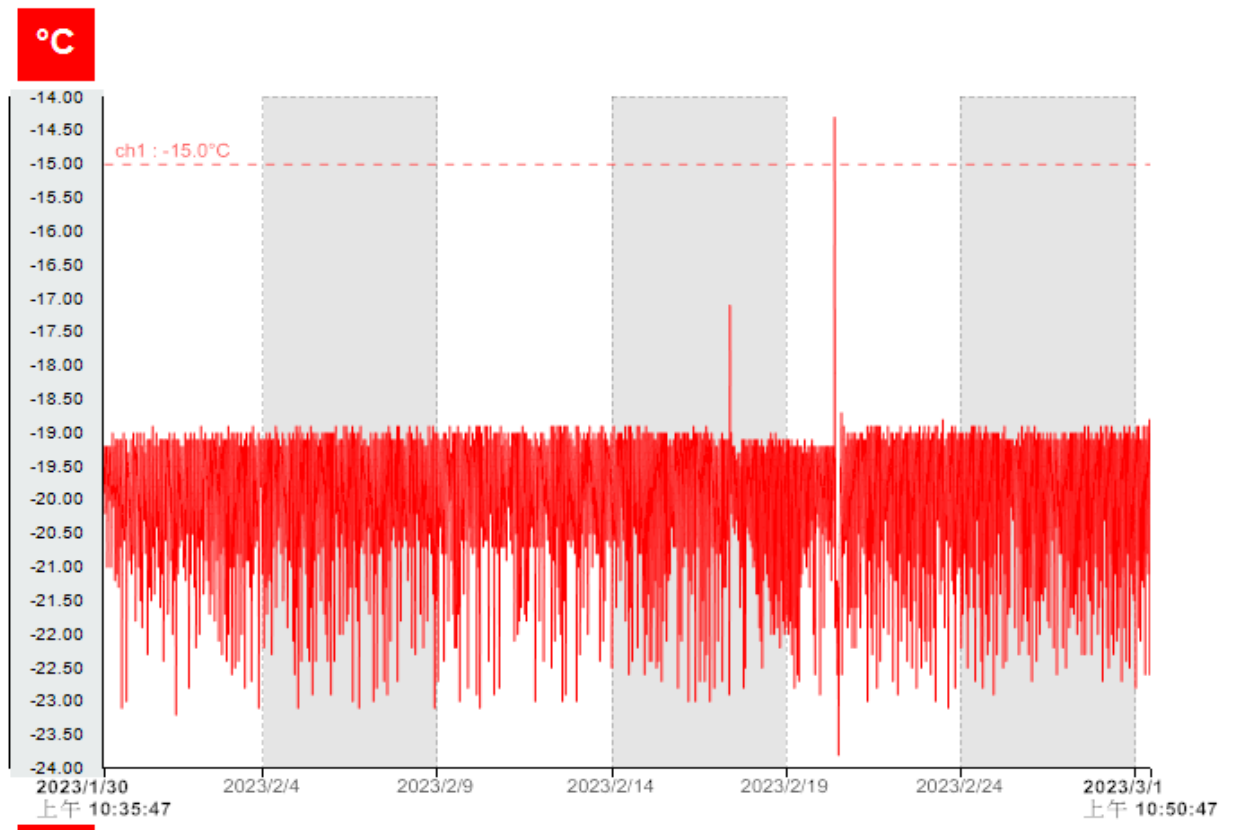

Comment: 2023年2月20日放置冰寶導致溫度暫時升高，目前未存放藥品。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 01, Mar 2023 ~ 31, Mar 2023



2K210923833

v1 [°C]				
Min	Max	Avg	Sd	MKT
-23.2	-18.7	-19.95	1.02	-19.88

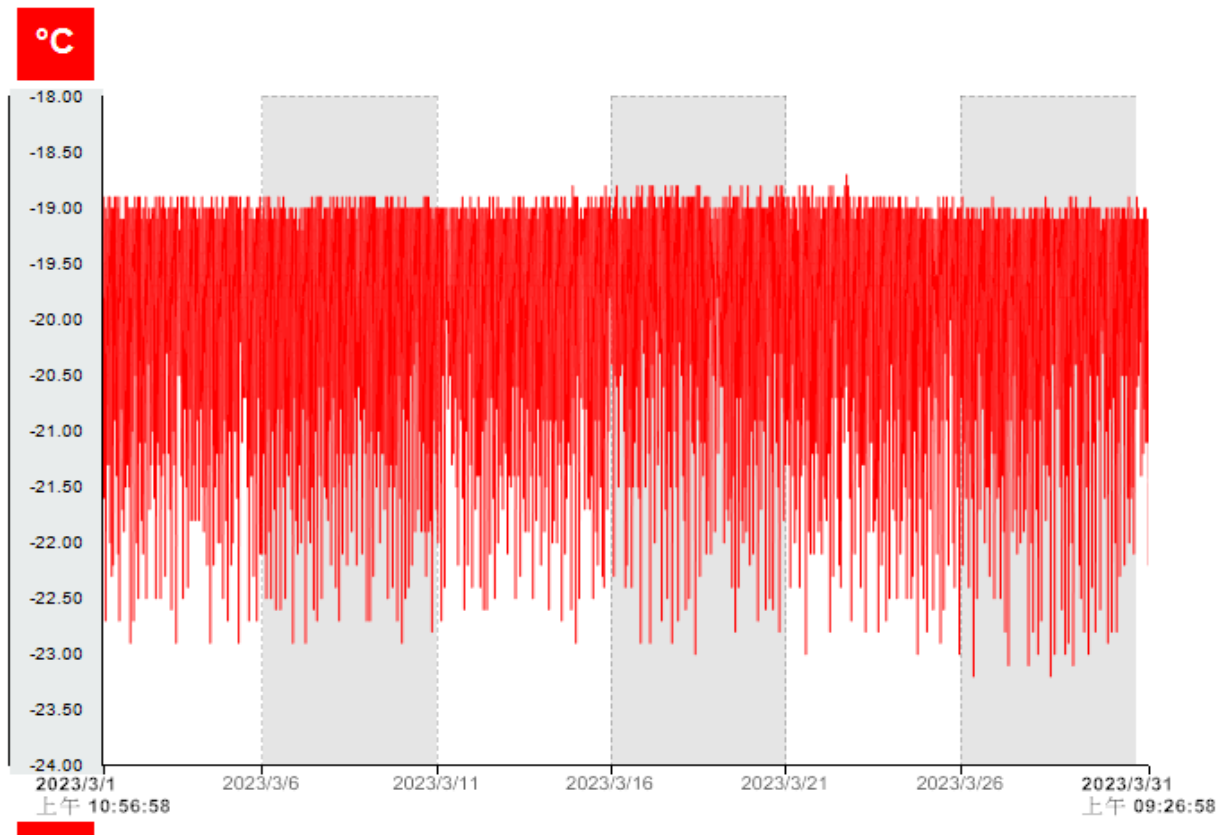

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Mar 2023 ~ 28, Apr 2023



2K210923833

v1 [°C]
Min Max Avg Sd MKT
-23.3 -18.9 -19.98 0.99 -19.91

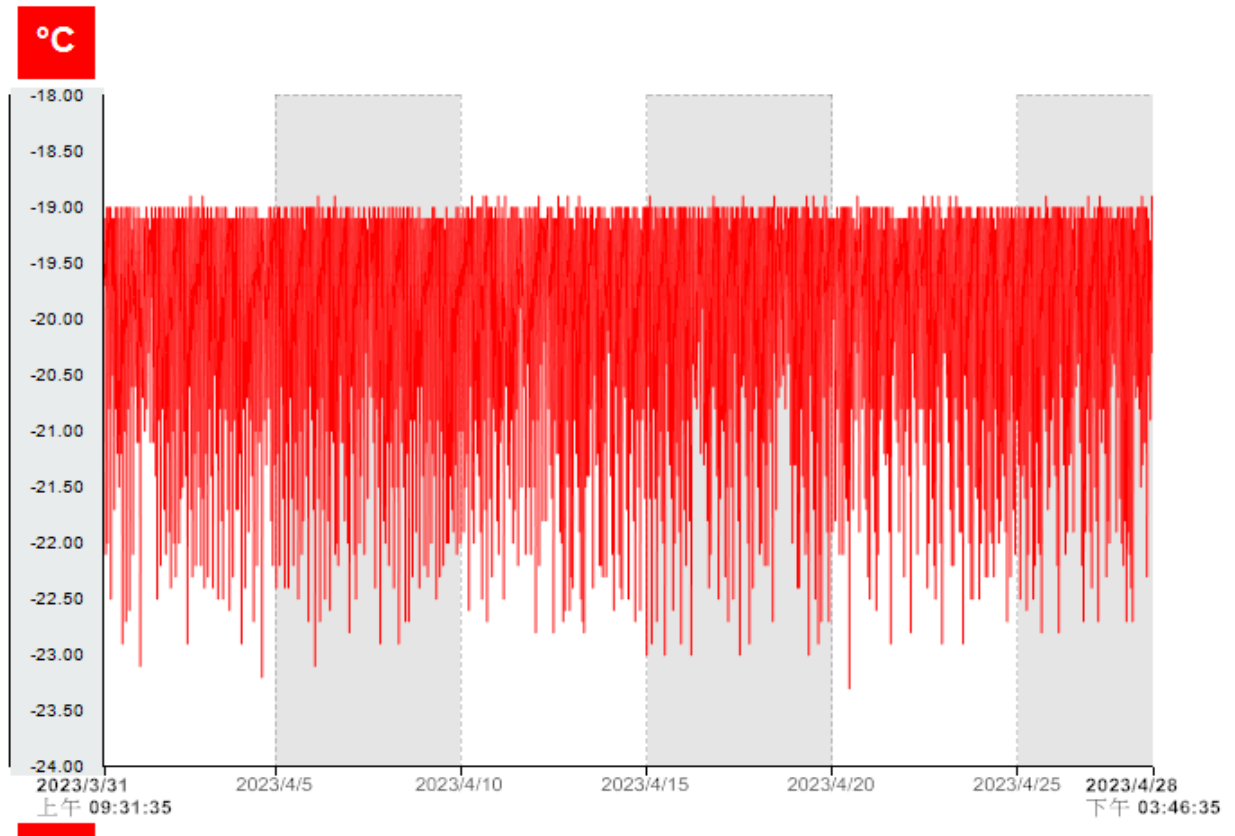

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top


THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 1D220605898; Channel No.: 1

FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 28, Apr 2023 ~ 29, May 2023



v1 [°C]
Min Max Avg Sd MKT
-23.1 -18.7 -19.85 0.95 -19.79

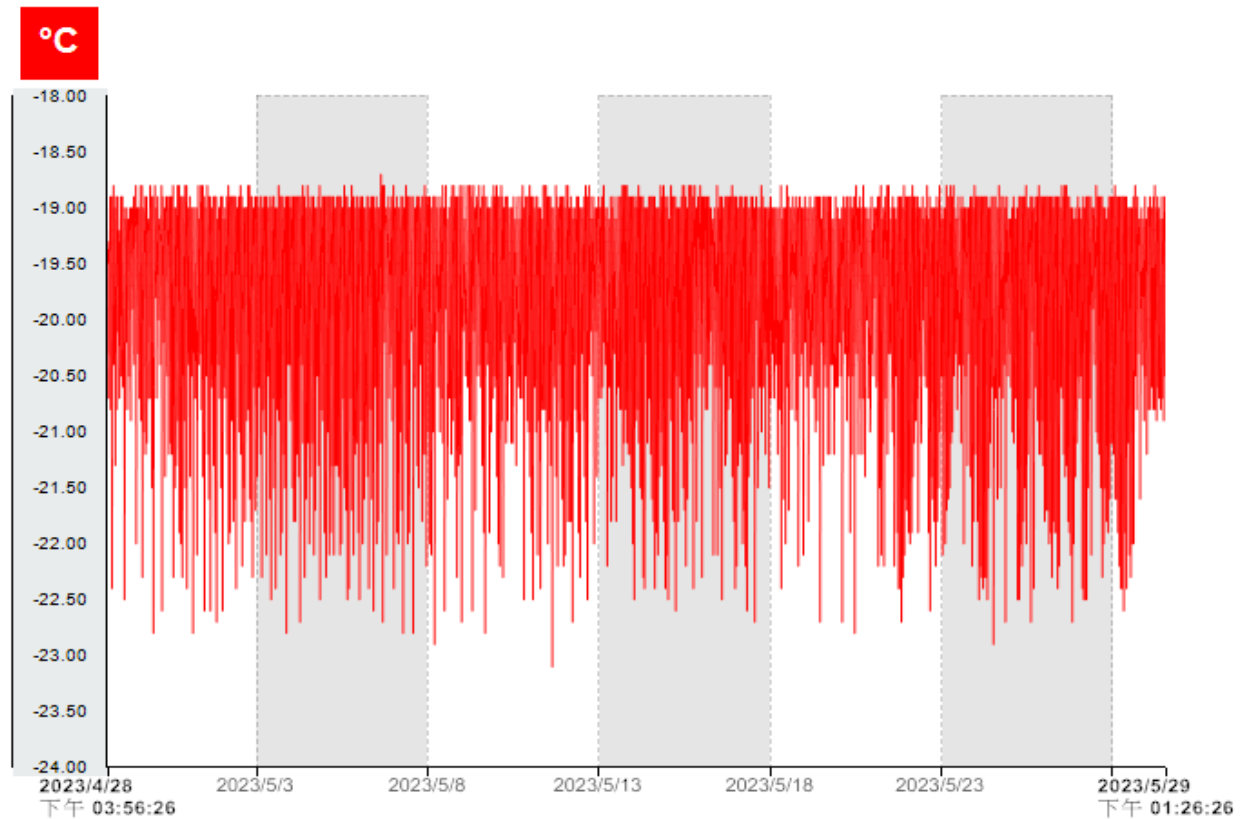

Comment: 本溫度記錄器(2K210923833)於2023年4月28日送校，期間以備品溫度記錄器(1D220605898)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : $-15\sim-25^{\circ}\text{C}$

DATE : 30, May 2023 ~ 30, Jun 2023



2K210923833

v1 [°C]
Min Max Avg Sd MKT
-22.8 -14.9 -19.68 0.82 -19.64

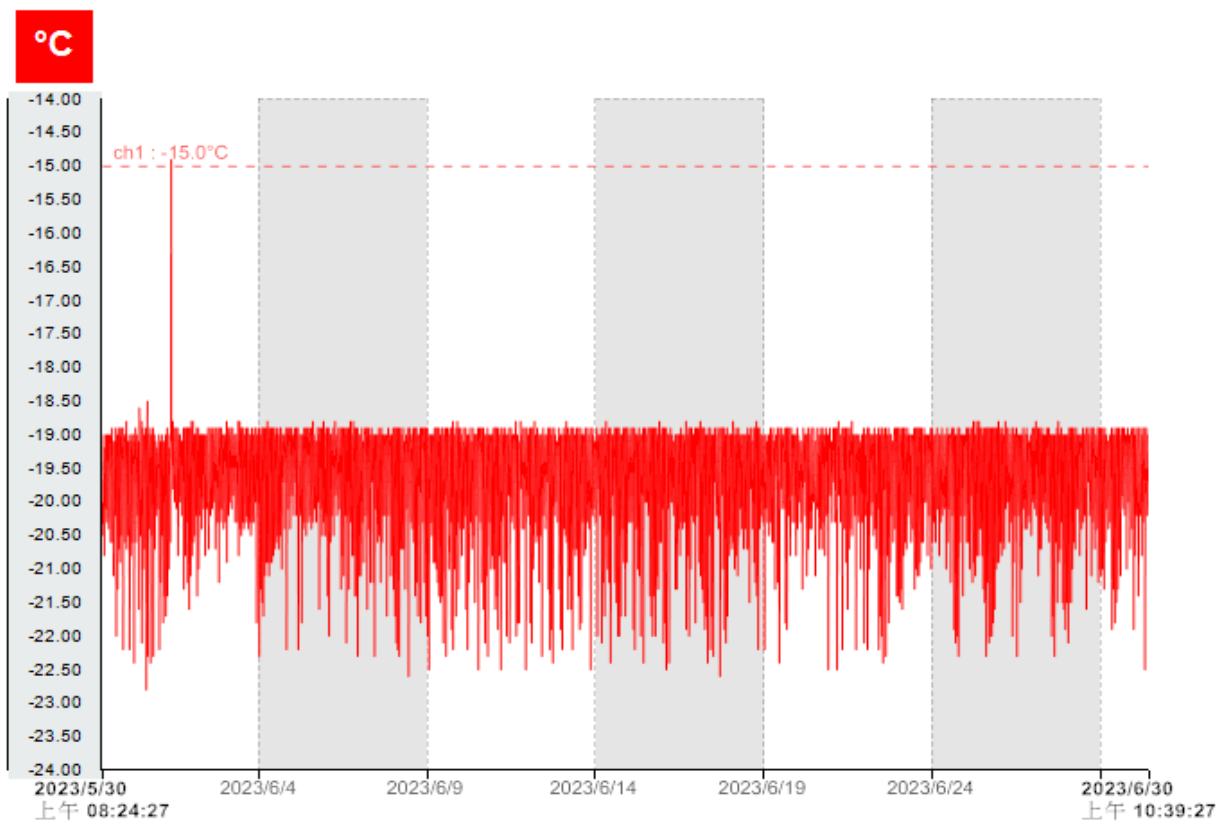

Comment: 於2023年5月29日13:30除霜，於2023年5月30日除霜完畢並於08:24重啟。2023年6月1日09:15空調人員檢查櫃體感溫線位置使暫時超溫，目前無存放藥品。本溫度記錄器(2K210923833)完成校正，於2023年5月30日換回使用。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Jun 2023 ~ 31, Jul 2023



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.8 -17.3 -19.72 0.87 -19.67

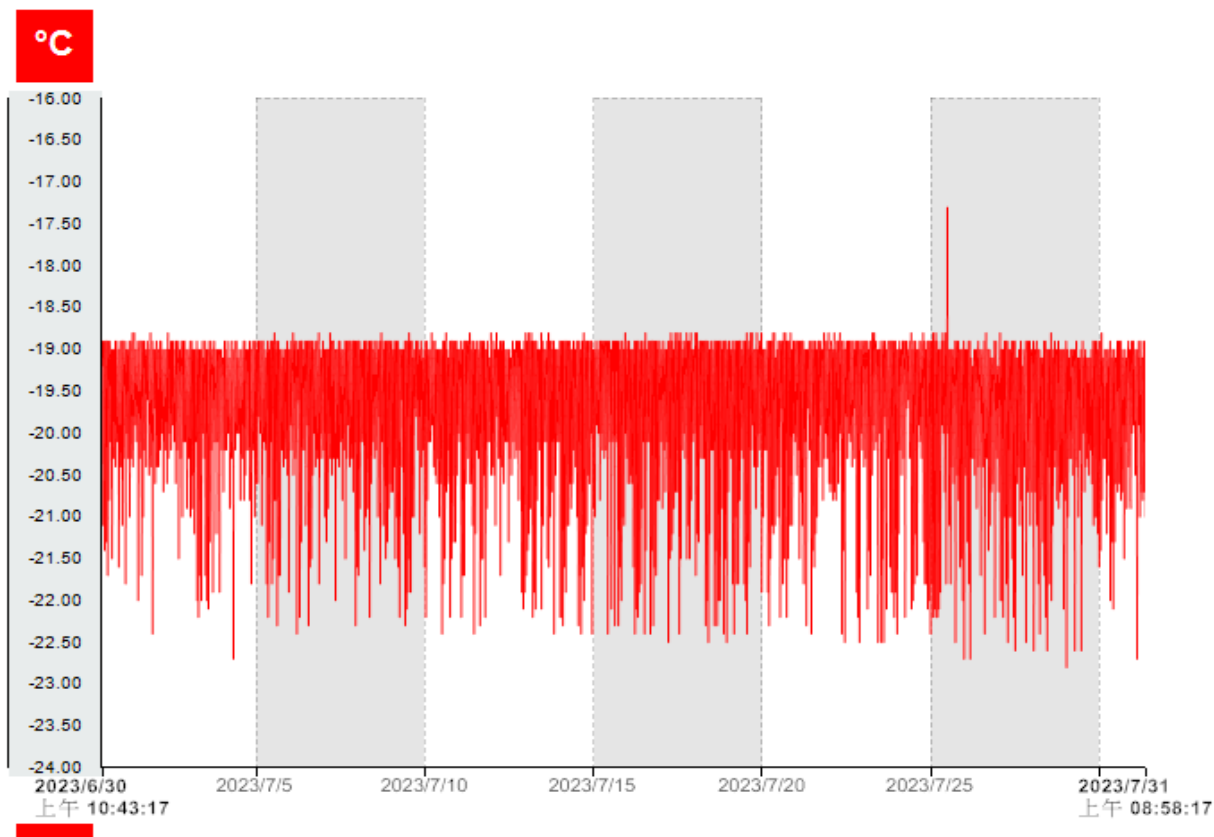

Comment: 因冷凍2下層須移動溫度記錄器的感溫線，本冷凍櫃（冷凍2上層）於2023年7月25日09:48開始儲存藥品，並於同日11:45將藥品移回冷凍2下層。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : $-15\sim-25^{\circ}\text{C}$

DATE : 31, Jul 2023 ~ 31, Aug 2023



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-23.0 -18.8 -19.74 0.78 -19.70

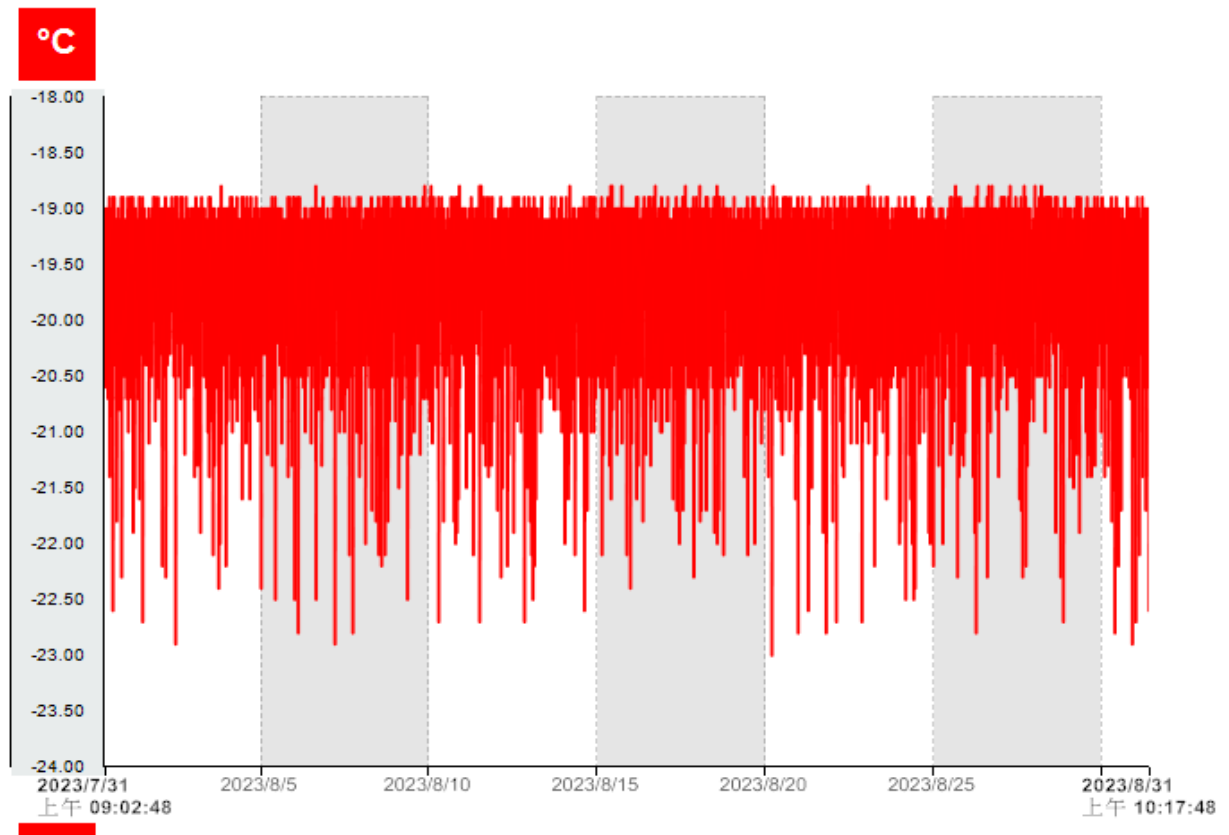

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Aug 2023 ~ 28, Sep 2023



2K210923833

v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.9 -14.7 -19.68 0.73 -19.64

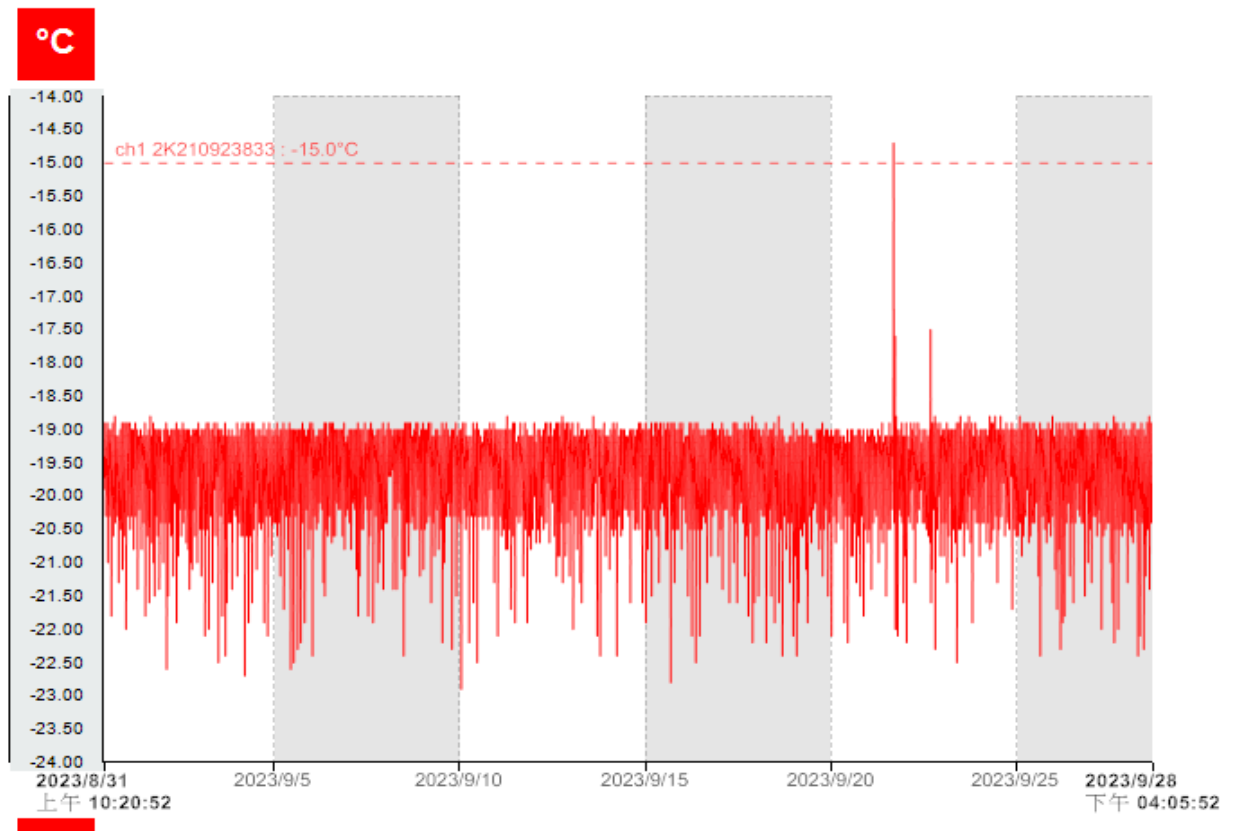

Comment: 於2023年9月21日16:00冰箱確效放置感溫線，暫時超溫。目前無存放藥品。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : $-15\sim-25^{\circ}\text{C}$

DATE : 28, Sep 2023 ~ 31, Oct 2023



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.8 -18.8 -19.74 0.71 -19.70

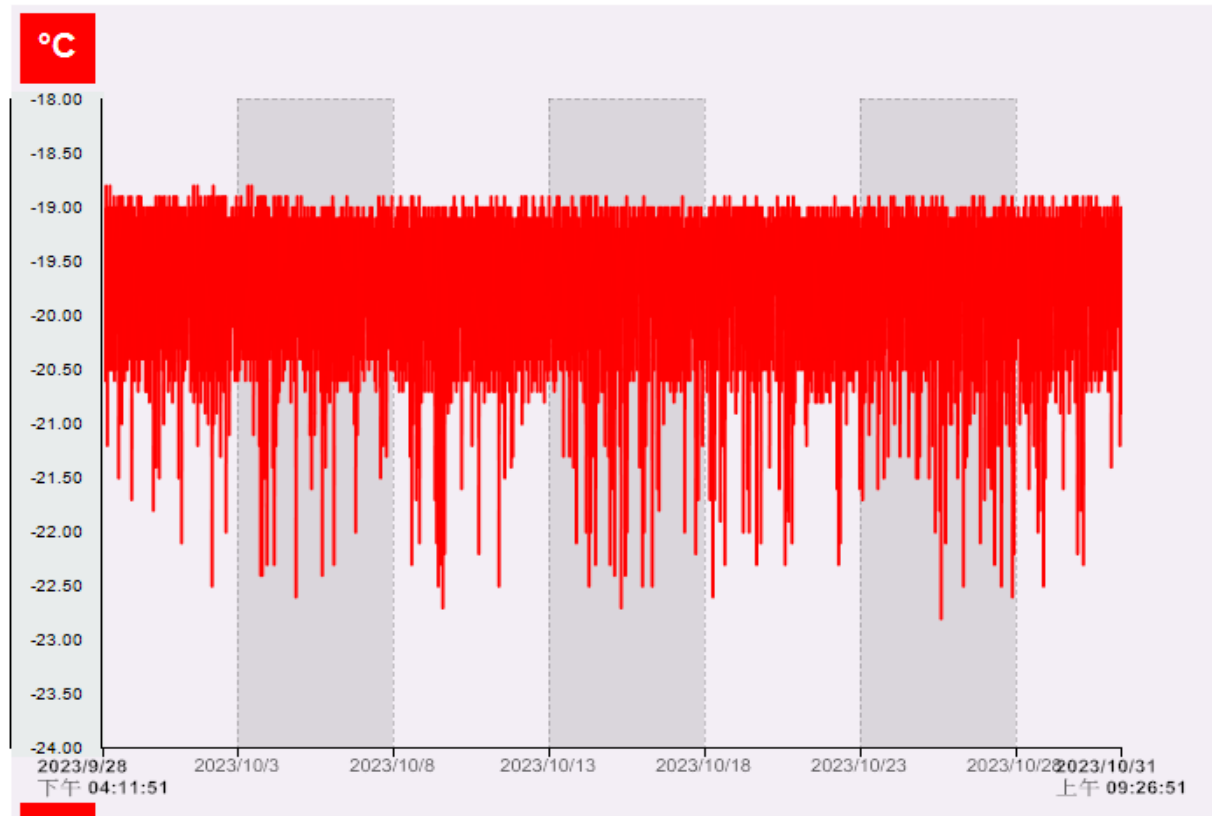

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Oct 2023 ~ 30, Nov 2023



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.6 -18.8 -19.72 0.65 -19.69

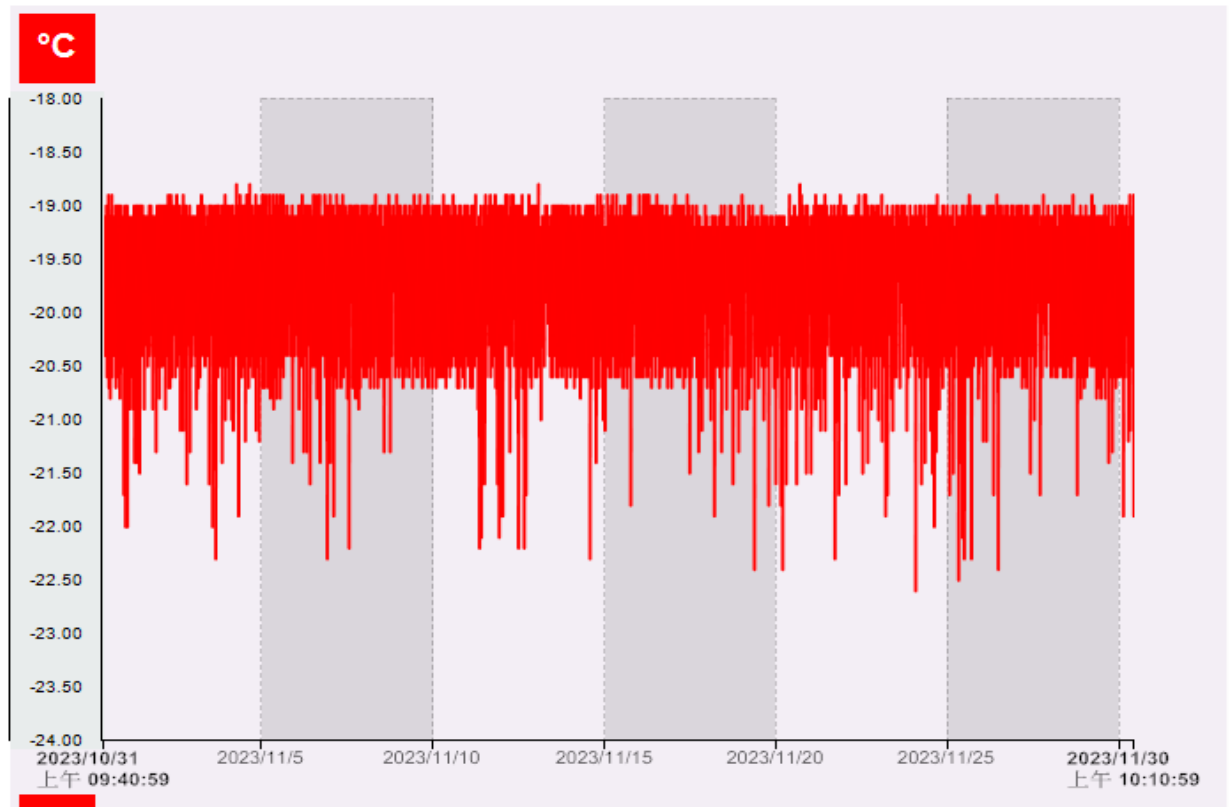

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 30, Nov 2023 ~ 29, Dec 2023



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.5 -18.9 -19.74 0.64 -19.71

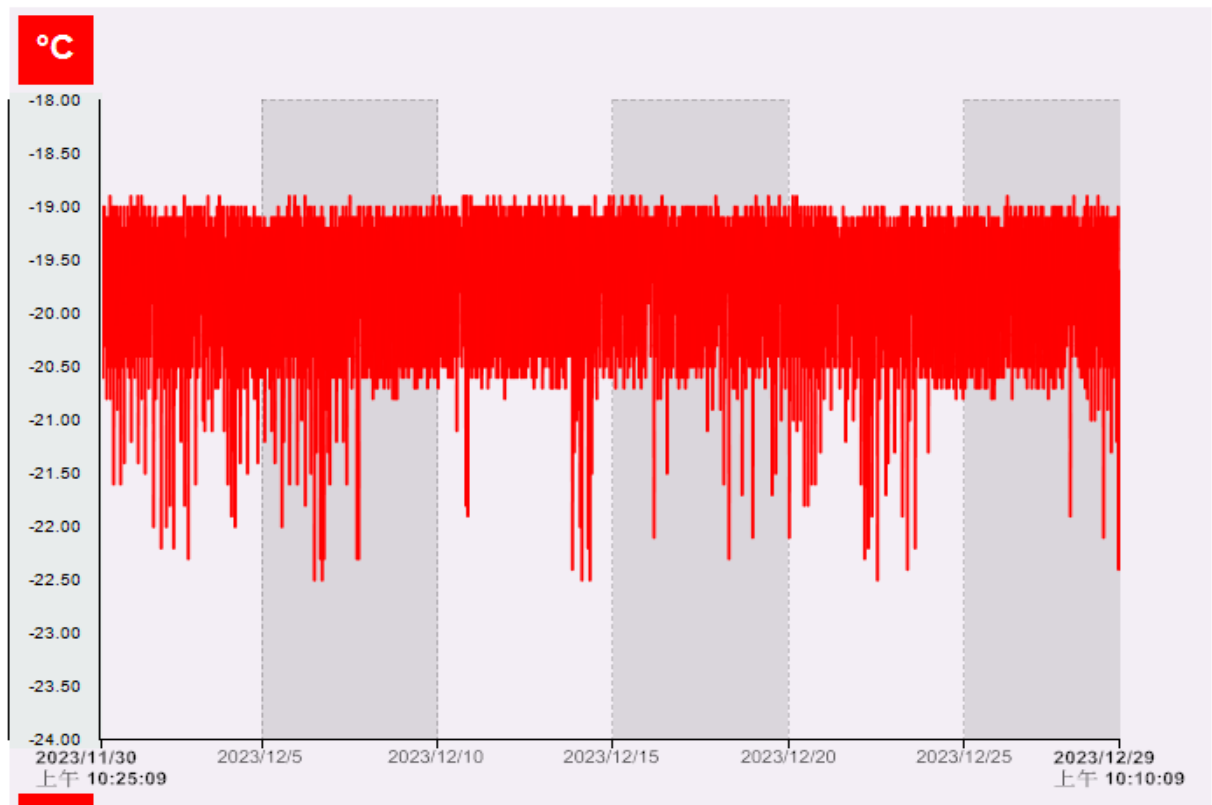

Comment: