

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 03, Jan 2023 ~ 30, Jan 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.9	5.8	4.52	0.45	4.53

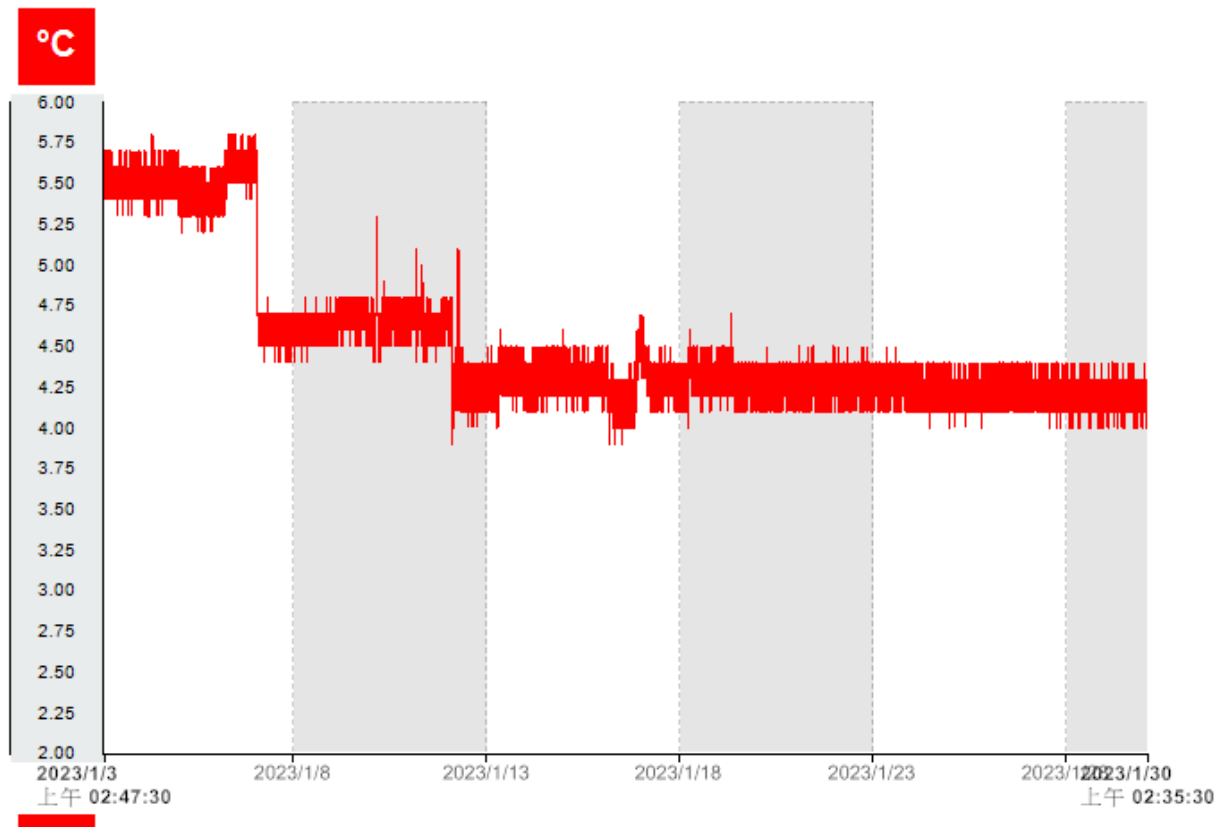

Comment: 因下載溫度用之筆電的時區有誤，此月份溫度記錄顯示之開始與結束時間比實際時間早8hr。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 30, Jan 2023 ~ 01, Mar 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.5	5.6	4.20	0.25	4.21

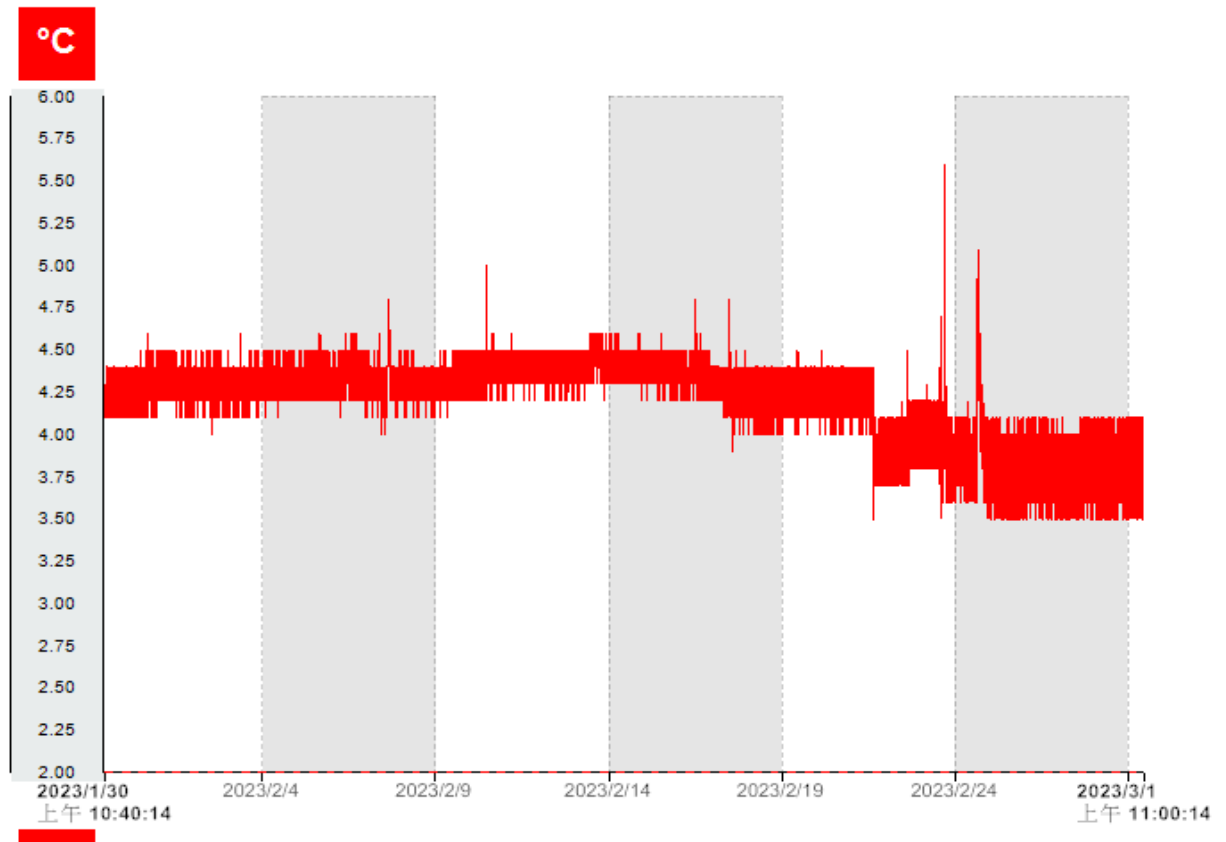

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 01, Mar 2023 ~ 31, Mar 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	5.2	3.87	0.21	3.87

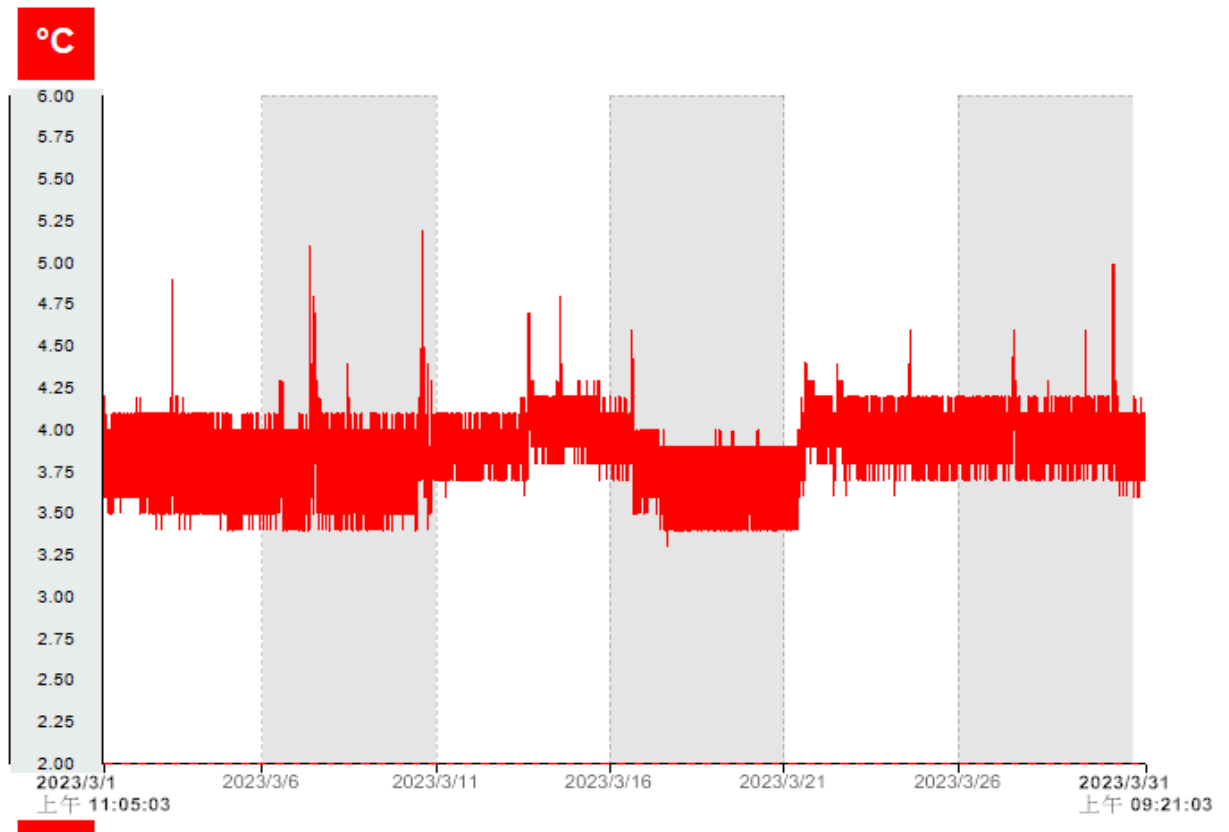

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 31, Mar 2023 ~ 28, Apr 2023



2K210923834

— v1 2K210923834 [°C]
Min Max Avg Sd MKT
3.5 5.6 4.11 0.21 4.11

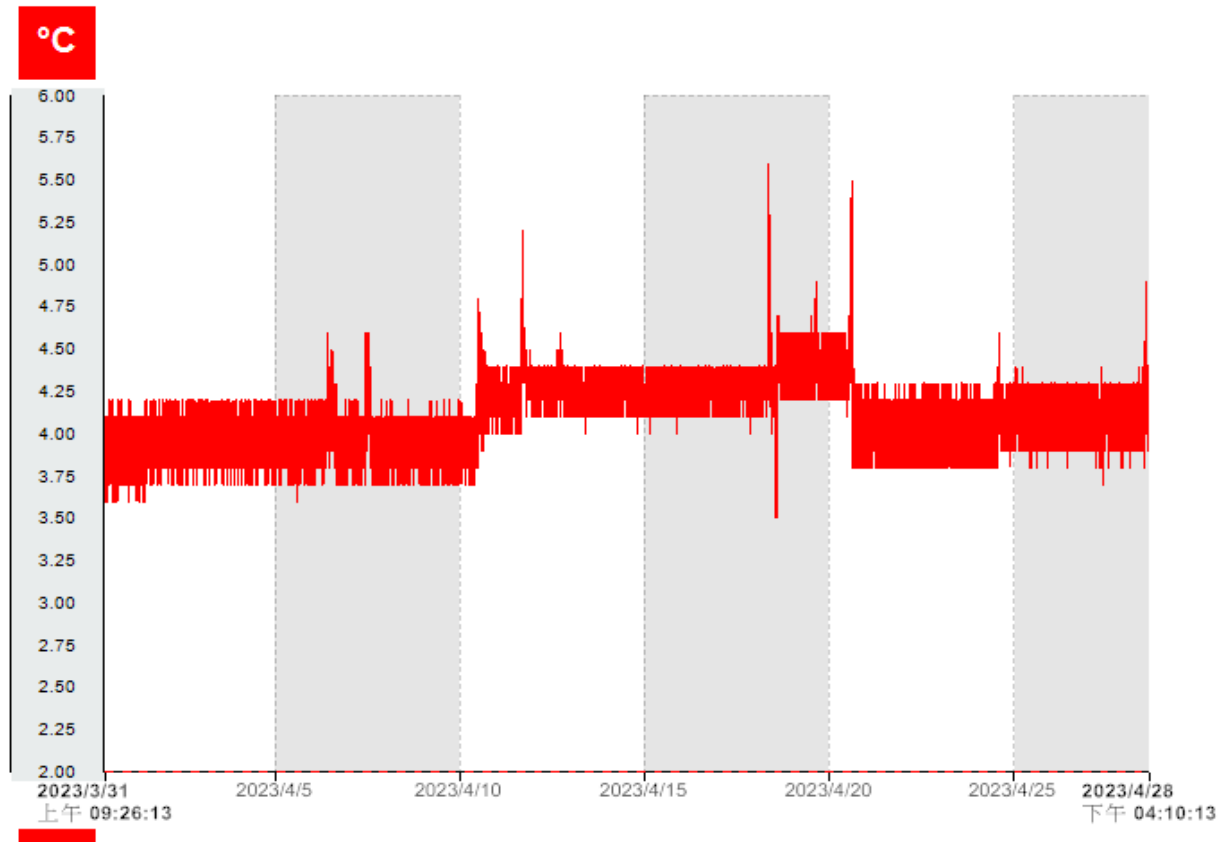

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 1D220605896; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 28, Apr 2023 ~ 29, May 2023



1D220605896

— v1 [°C]
Min Max Avg Sd MKT
2.8 5.6 4.46 0.18 4.46

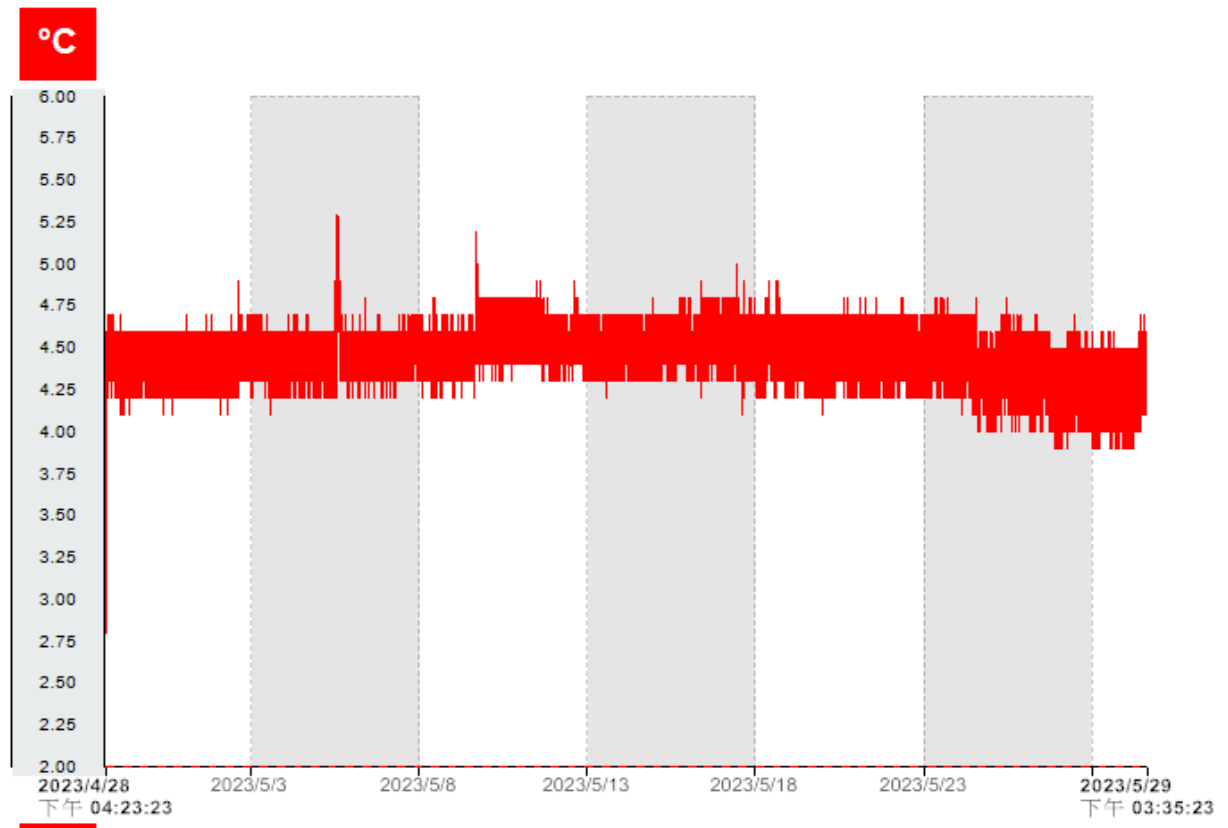

Comment: 本溫度記錄器(2K210923834)於2023年4月28日送校，期間以備品溫度記錄器(1D220605896)暫代。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 29, May 2023 ~ 30, Jun 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	6.0	4.47	0.47	4.48

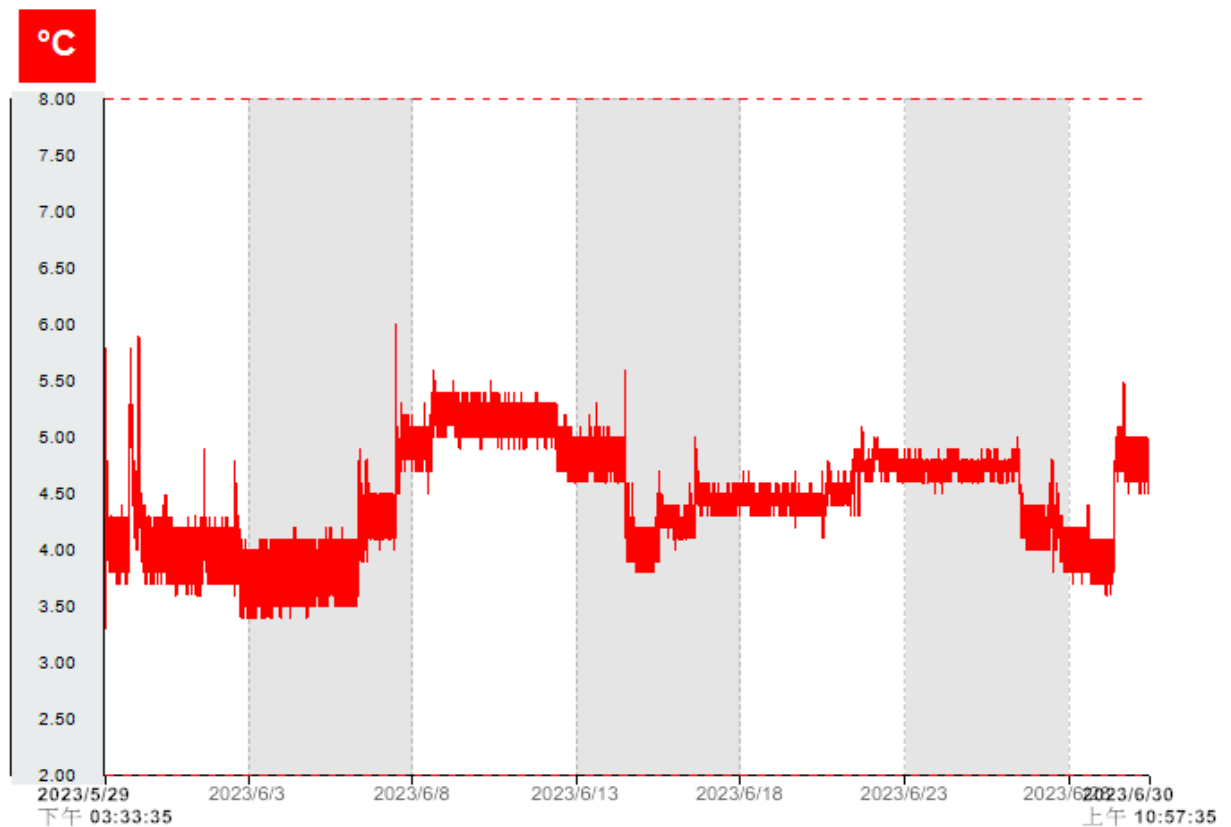

Comment: 本溫度記錄器(2K210923834)完成校正，於2023年5月29日換回使用。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 30, Jun 2023 ~ 31, Jul 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.7	6.3	4.48	0.23	4.48

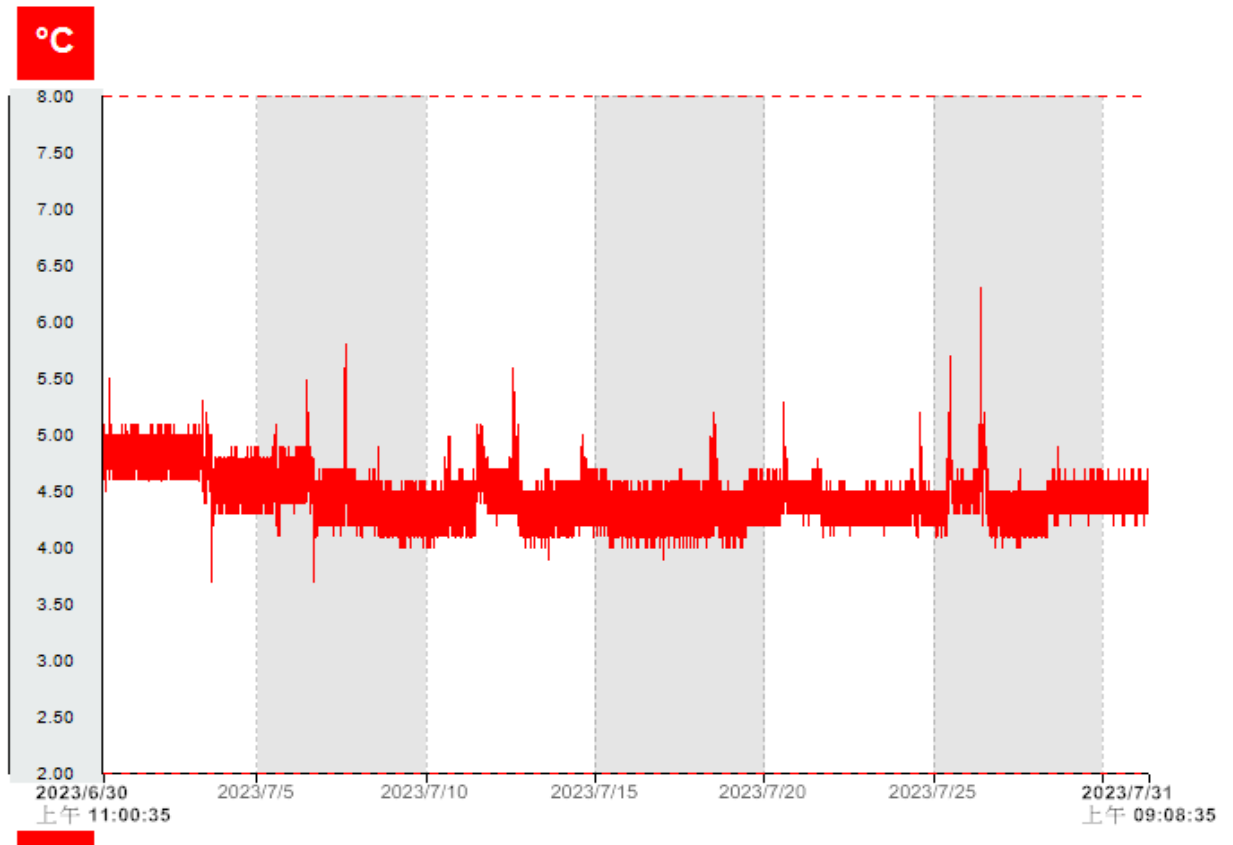

Comment:

/

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 31, Jul 2023 ~ 31, Aug 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.5	6.8	4.55	0.17	4.55

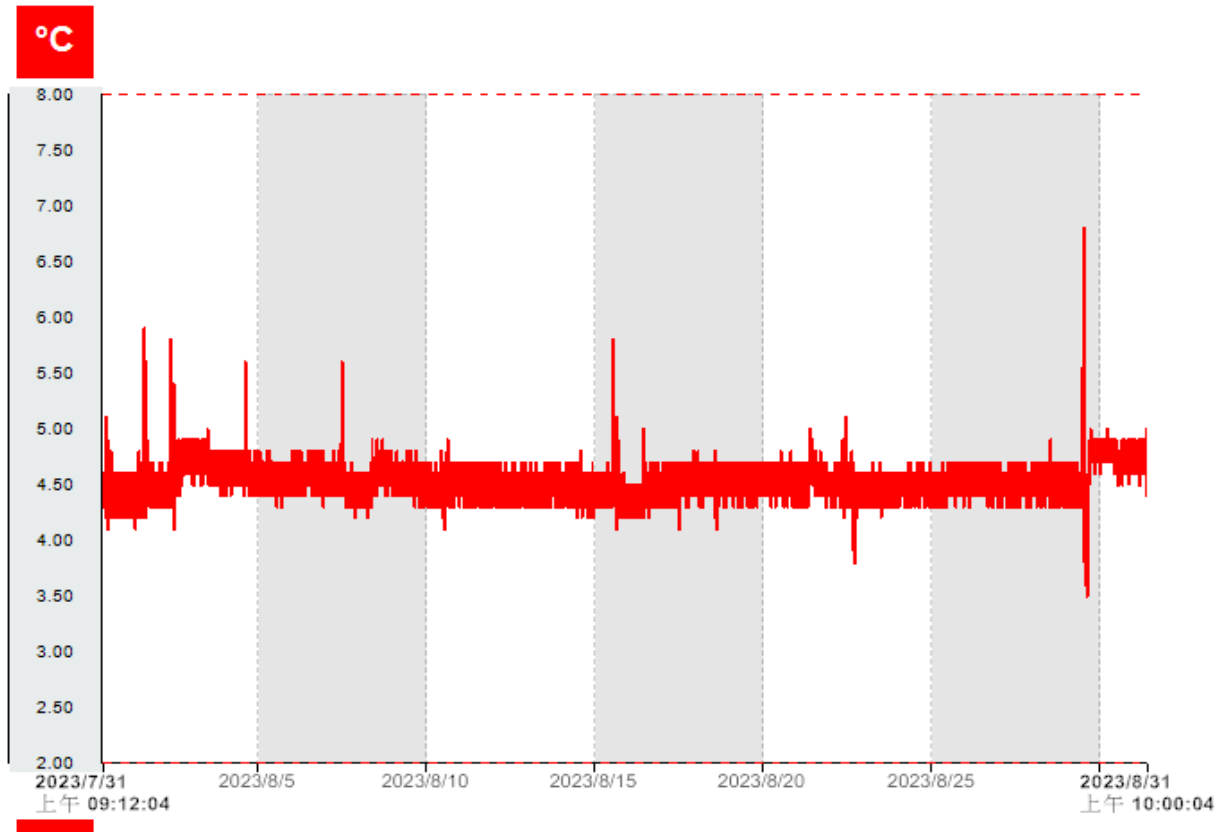

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 31, Aug 2023 ~ 28, Sep 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.2	6.1	4.34	0.25	4.34

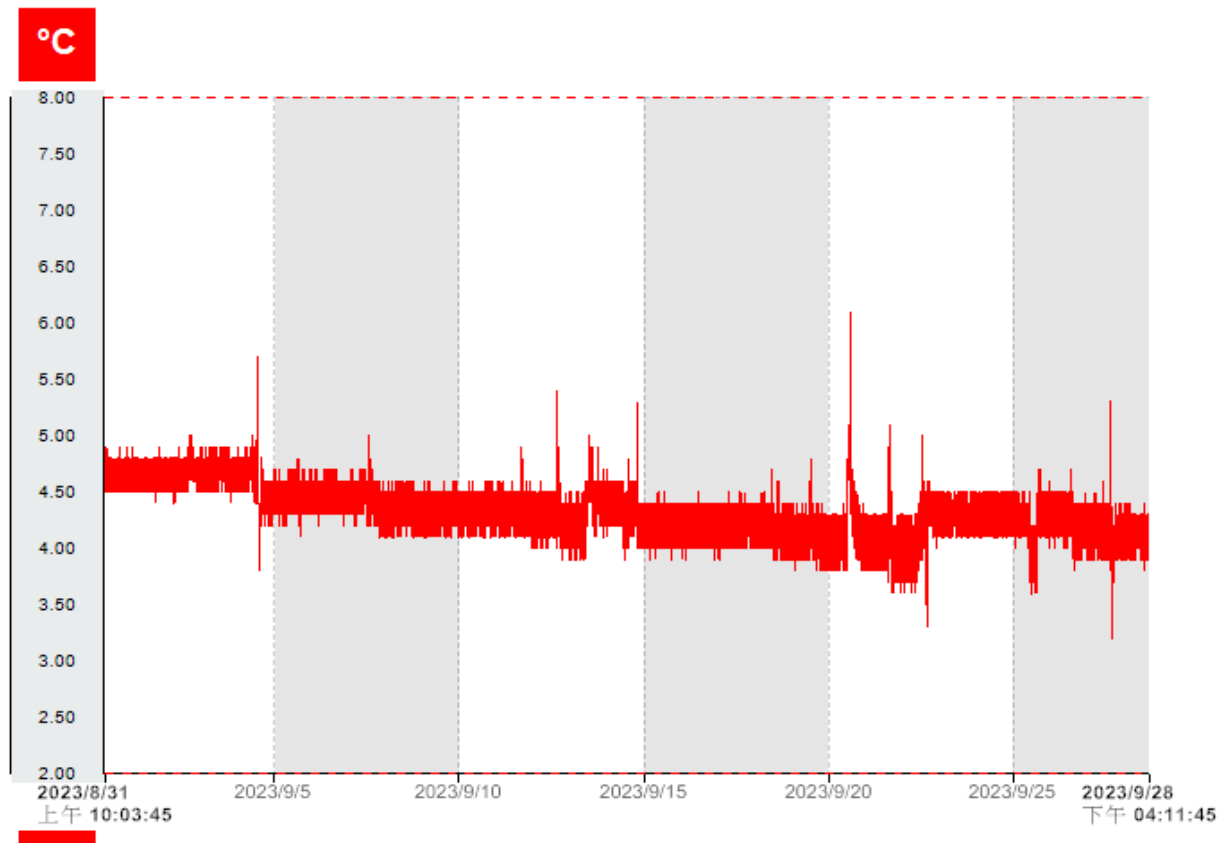

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 28, Sep 2023 ~ 31, Oct 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.6	5.6	4.29	0.18	4.30

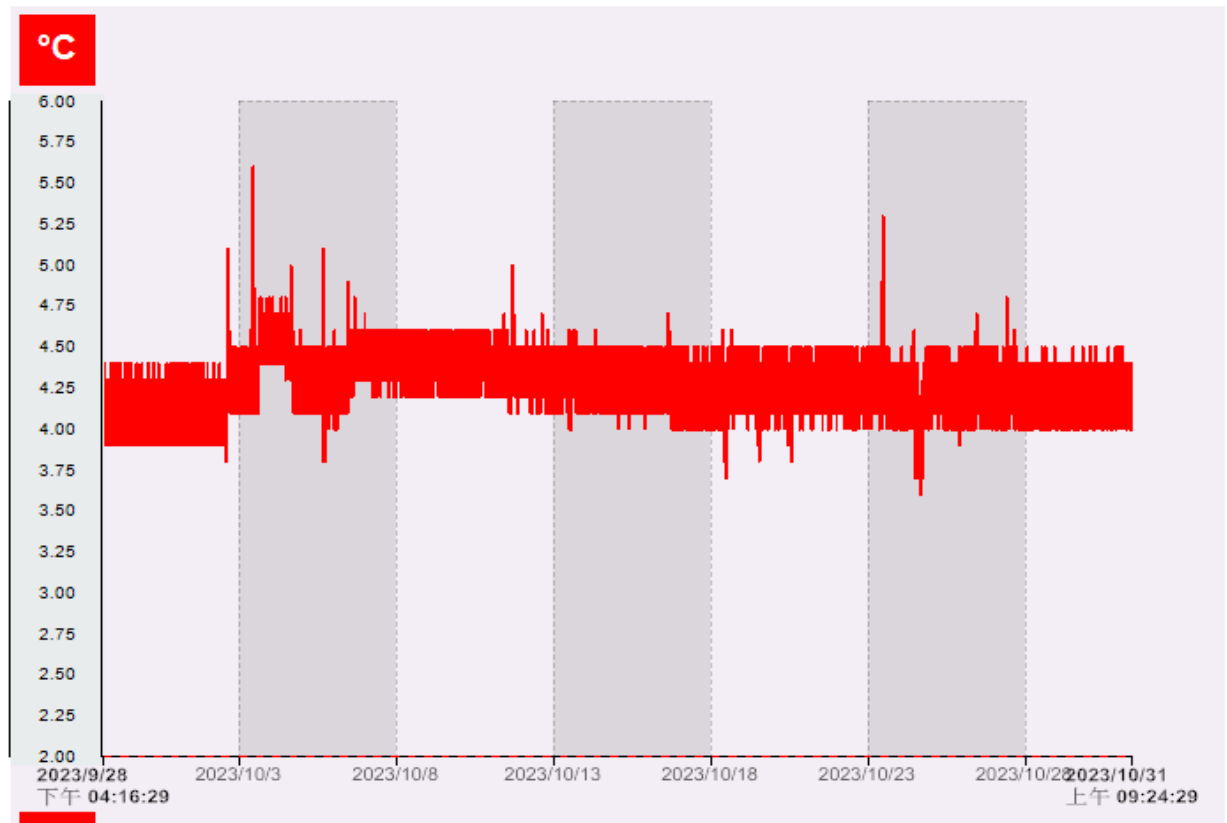

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 31, Oct 2023 ~ 2, Nov 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.7	5.4	4.22	0.28	4.22

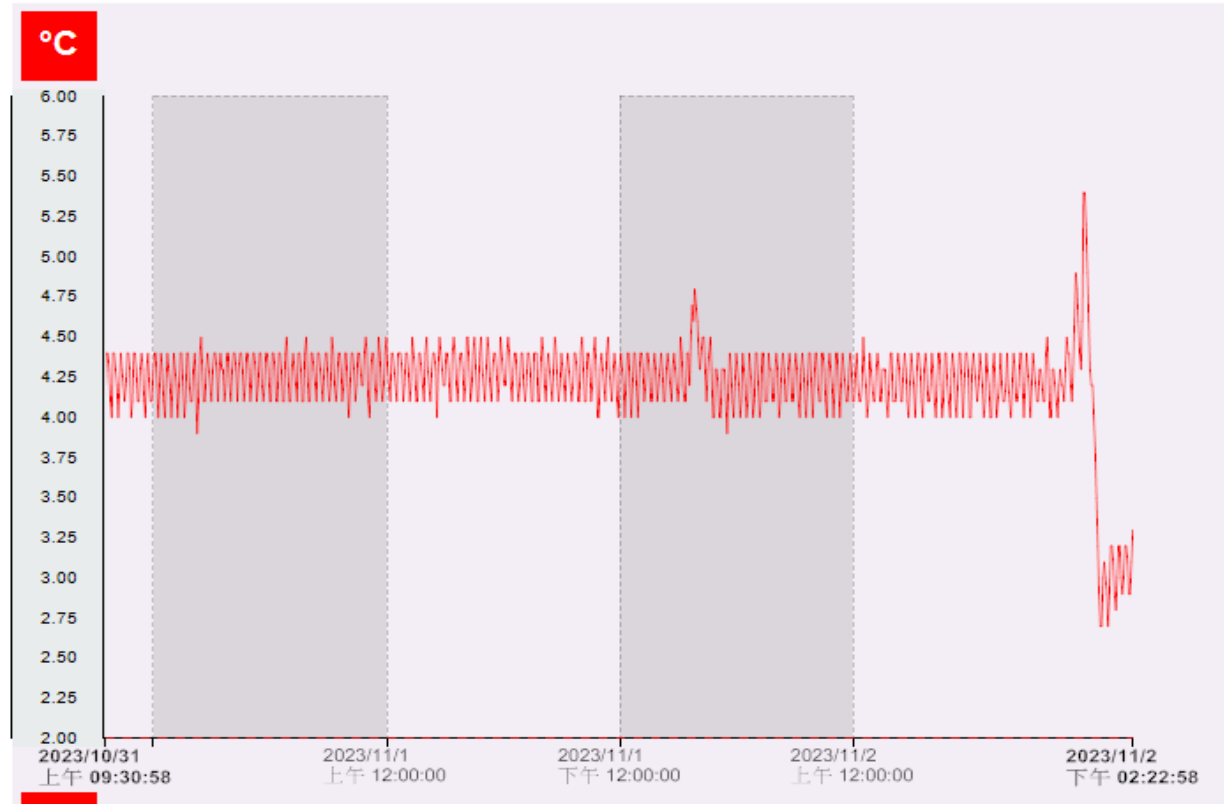

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 2, Nov 2023 ~ 3, Nov 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
2.8	4.3	3.91	0.23	3.92

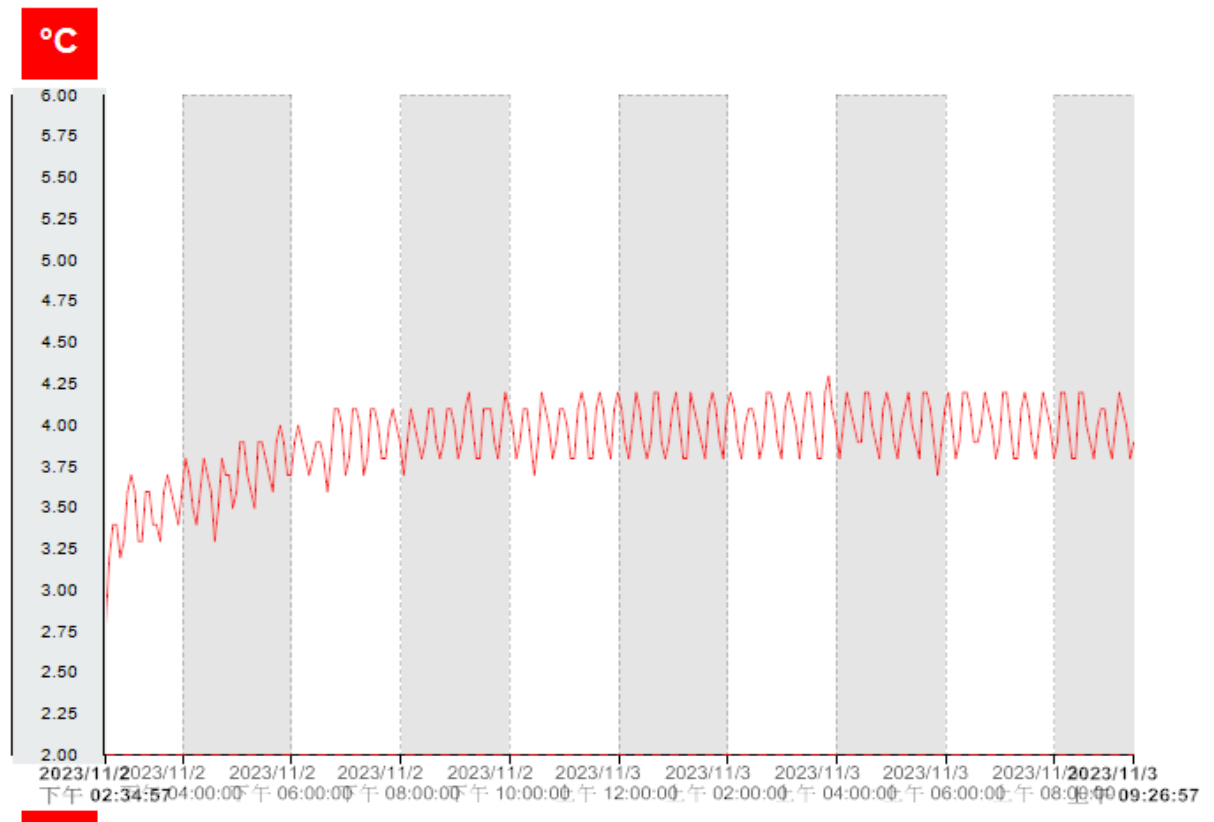

Comment: 於2023年11月3日更換溫度記錄器的感溫線，調整感溫探頭後重啟。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 3, Nov 2023 ~ 30, Nov 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.3	5.5	4.11	0.32	4.12

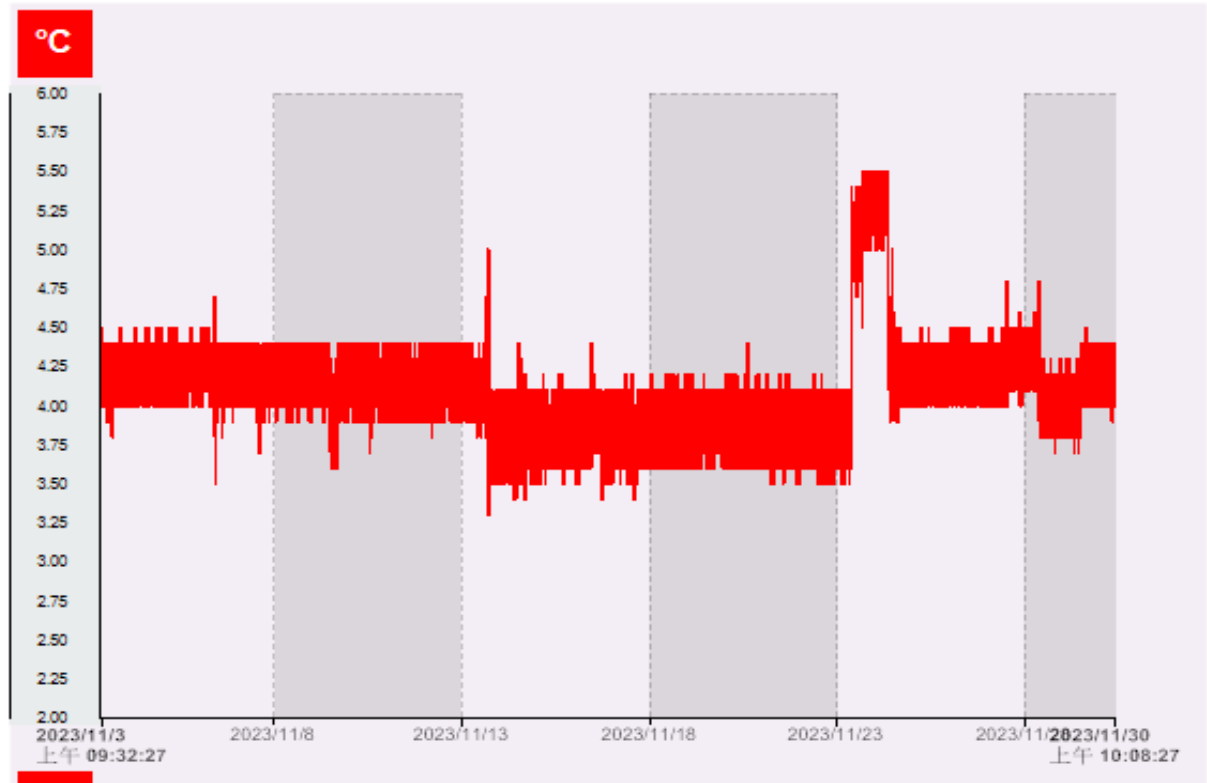

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 30, Nov 2023 ~ 29, Dec 2023



2K210923834

v1 [°C]				
Min	Max	Avg	Sd	MKT
3.2	4.9	3.99	0.19	4.00

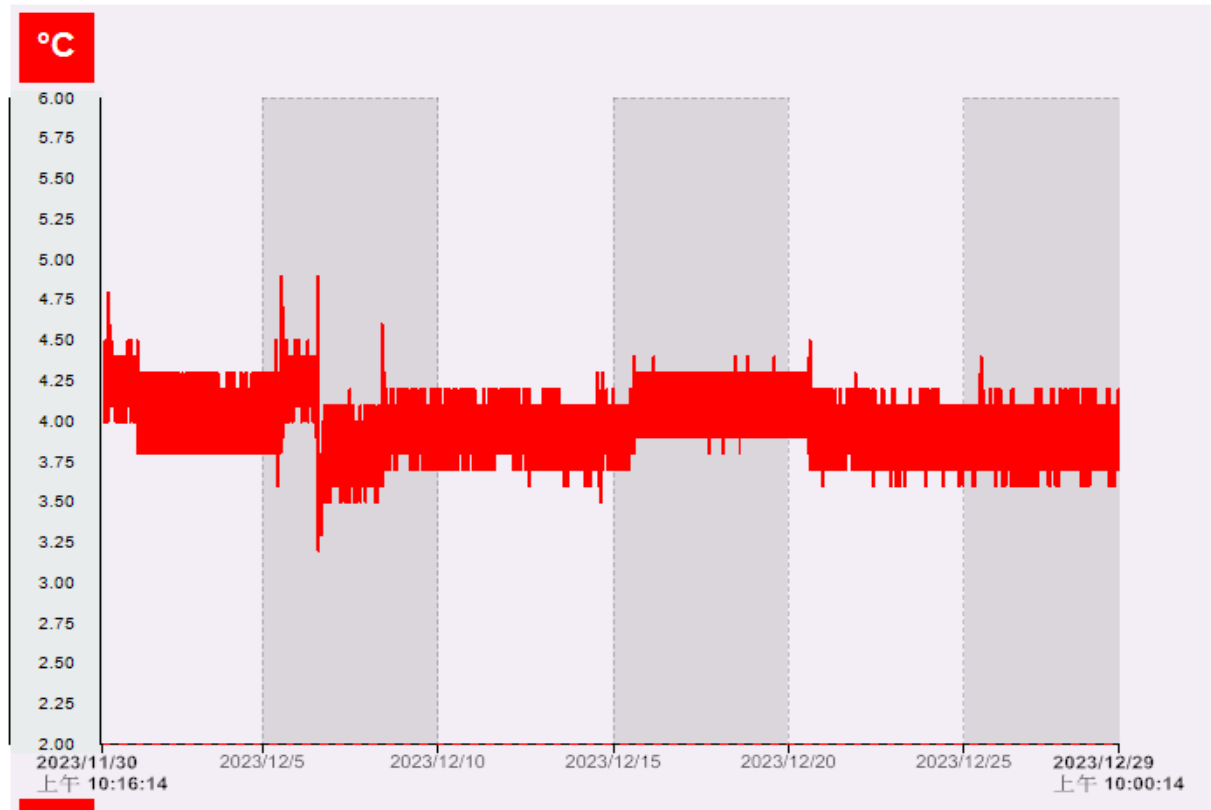

Comment: