

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 03, Jan 2023 ~ 30, Jan 2023



**KIMO 2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
3.2 4.9 4.15 0.25 4.15

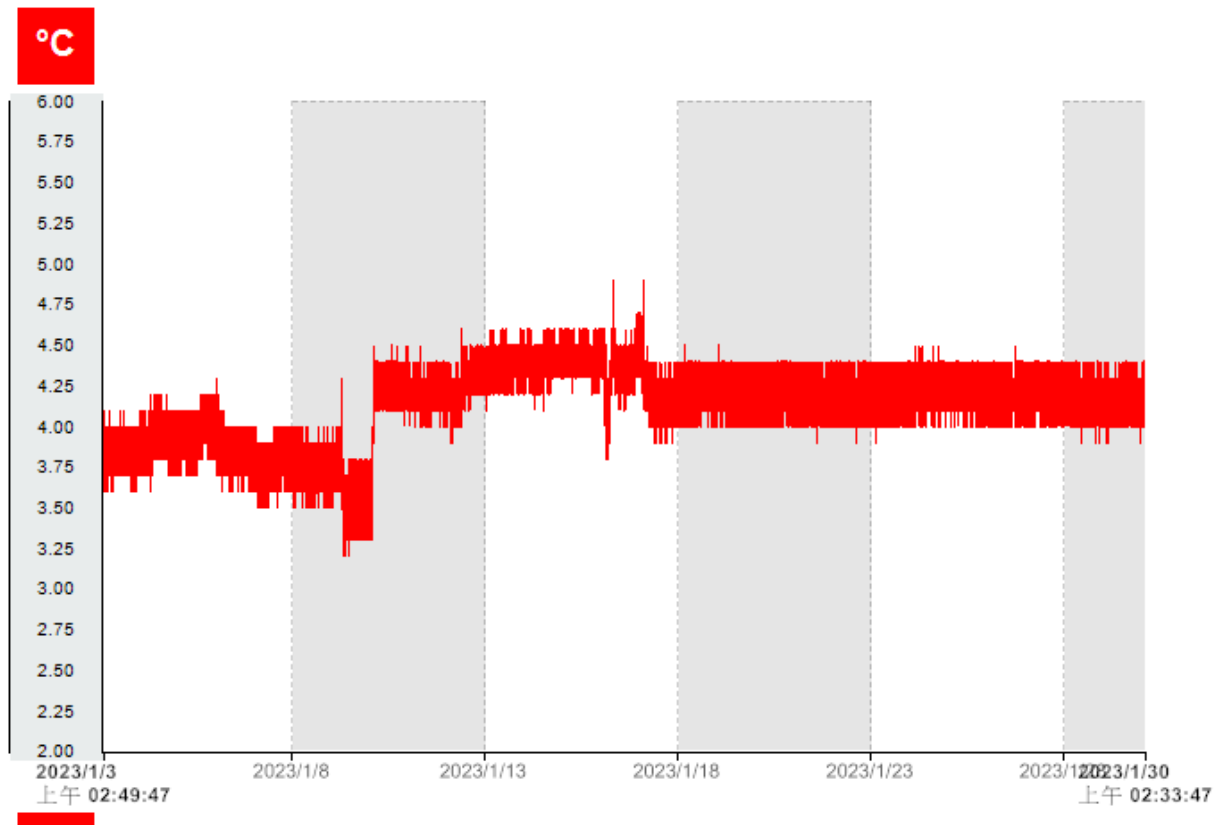

Comment: 因下載溫度用之筆電的時區有誤，此月份溫度記錄顯示之開始與結束時間比實際時間早8hr。

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 30, Jan 2023 ~ 01, Mar 2023



**KIMO 2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
3.6 6.0 4.38 0.23 4.38

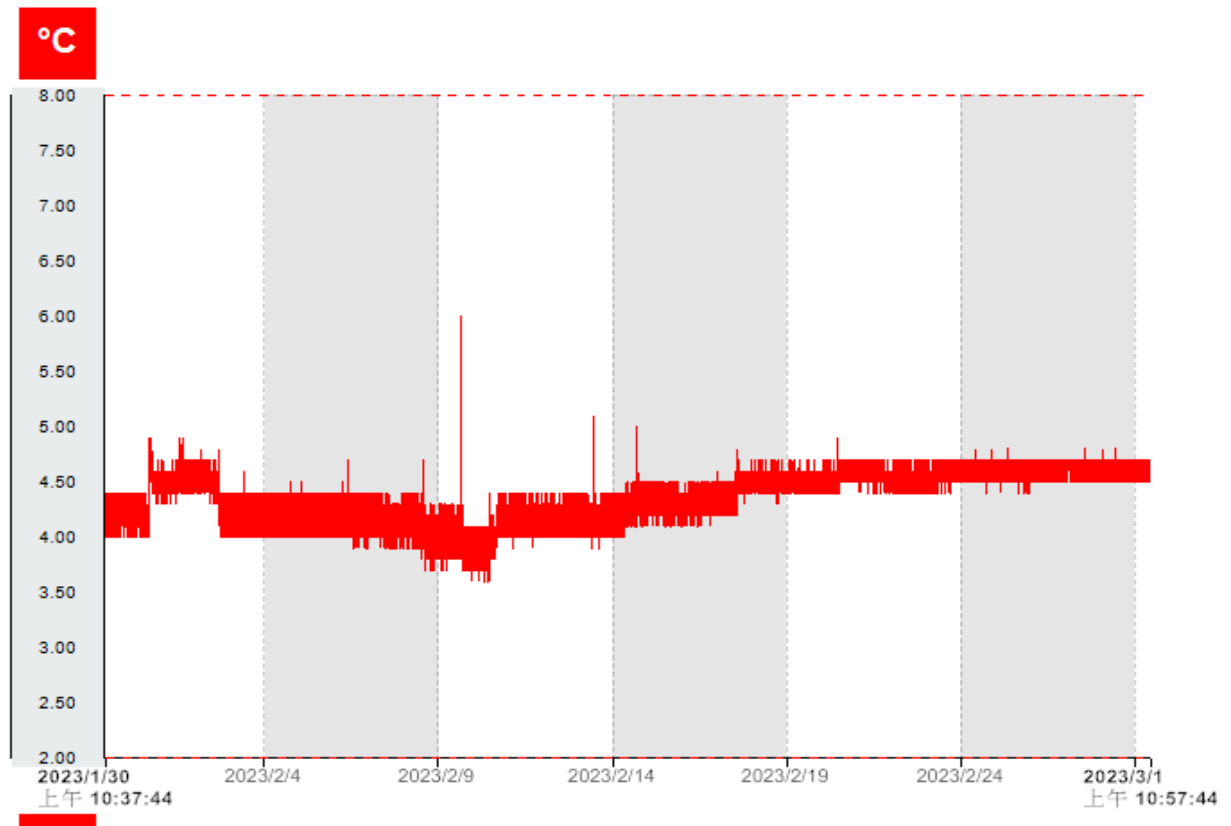

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022


**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1

**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 01, Mar 2023 ~ 31, Mar 2023



**2K190616069**

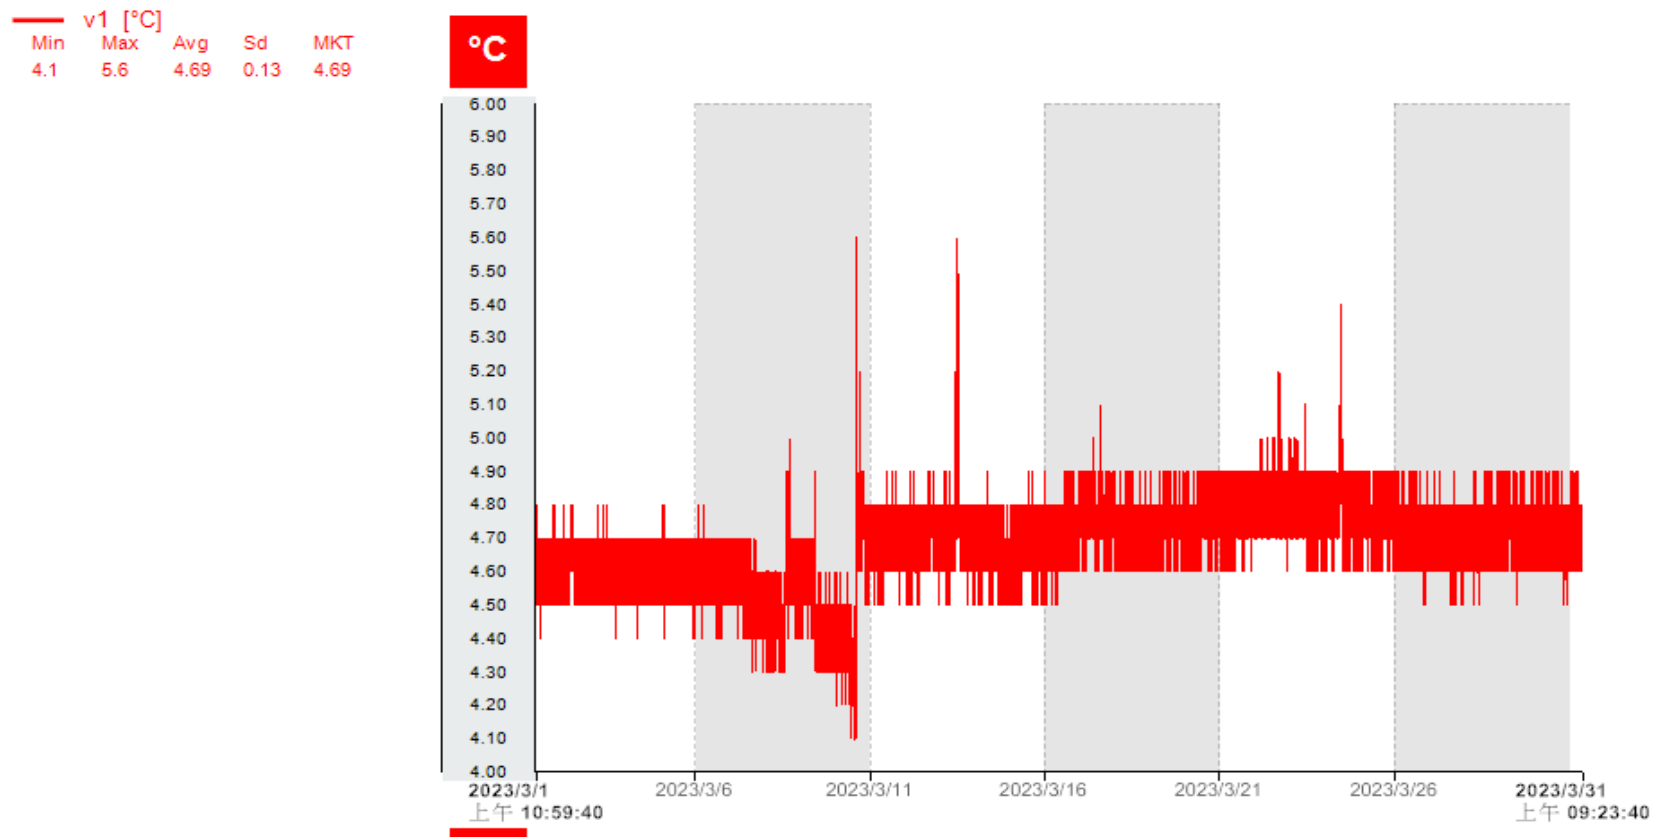

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 31, Mar 2023 ~ 28, Apr 2023



**2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
4.1 6.0 4.74 0.21 4.75

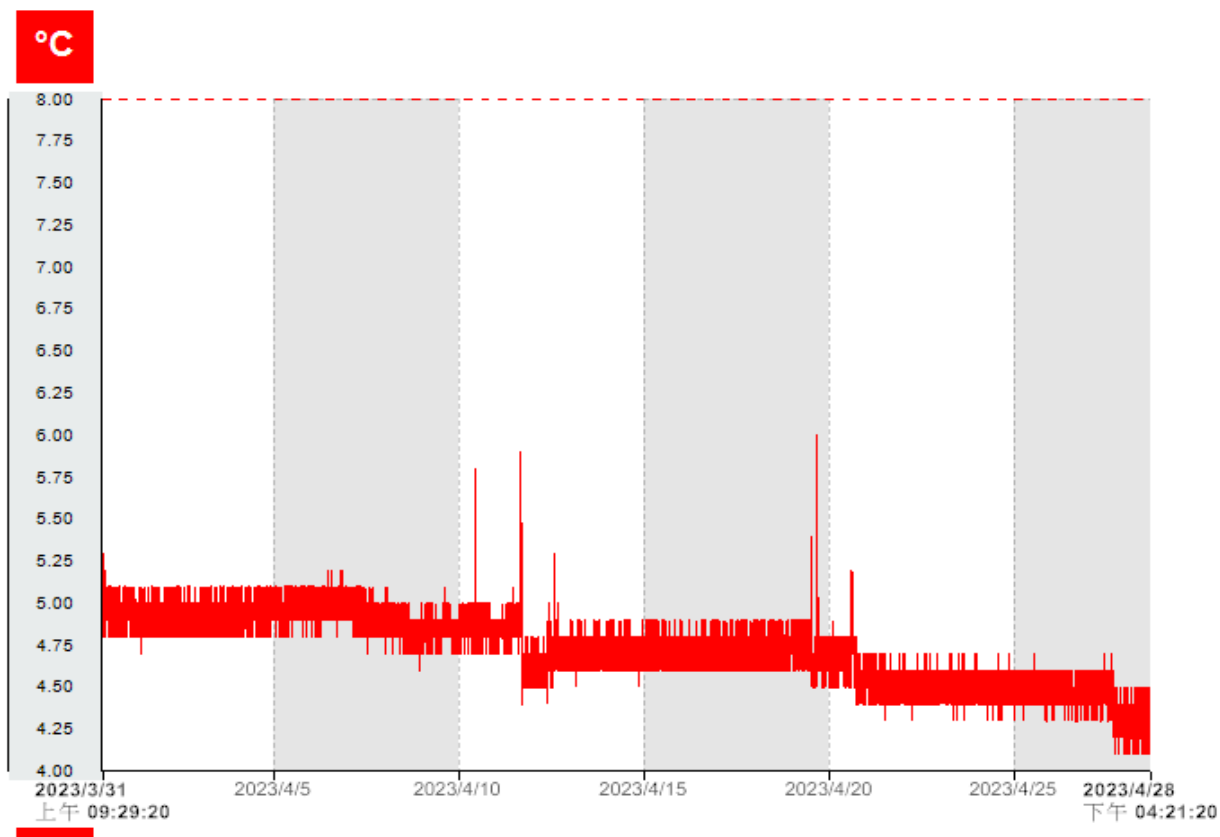

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 28, Apr 2023 ~ 29, May 2023



**2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
3.9 5.5 4.54 0.18 4.54

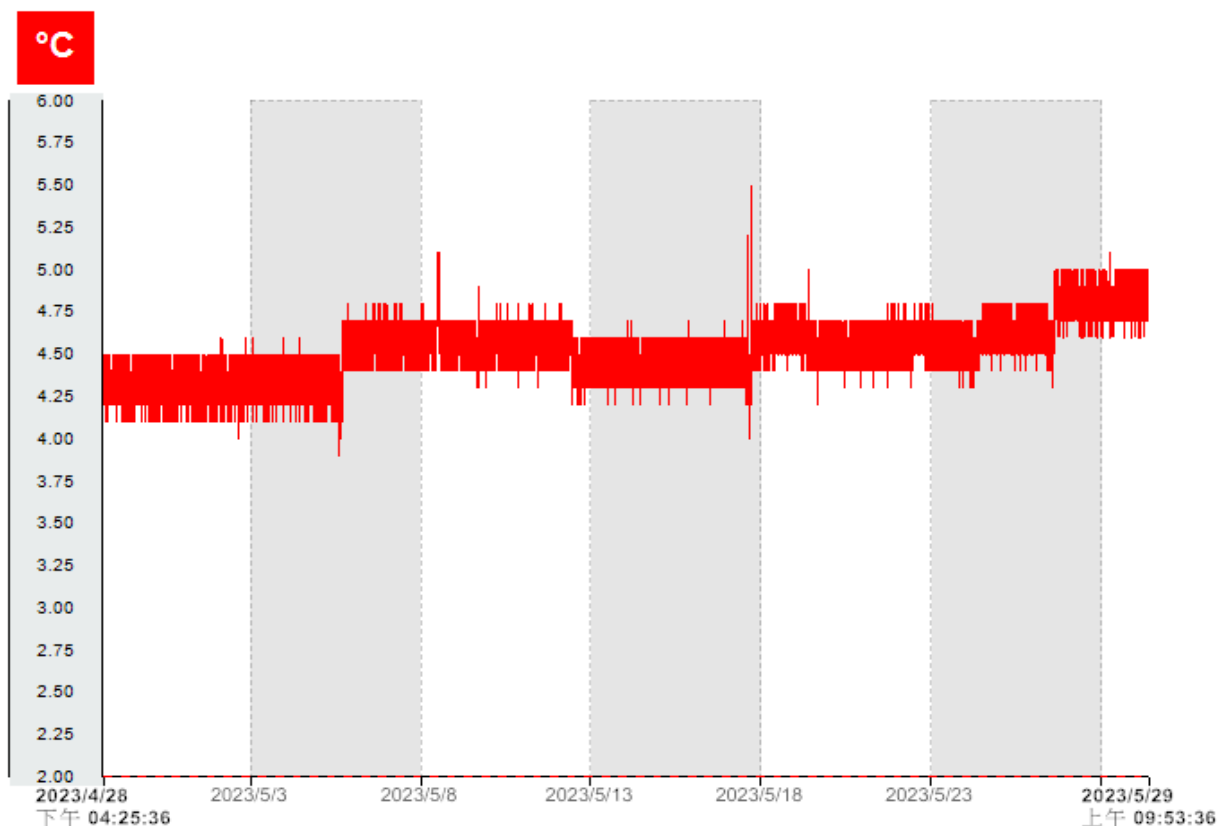

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 29, May 2023 ~ 14, Jun 2023



2K190616069

— v1 [°C]  
Min Max Avg Sd MKT  
3.8 5.9 4.61 0.18 4.61

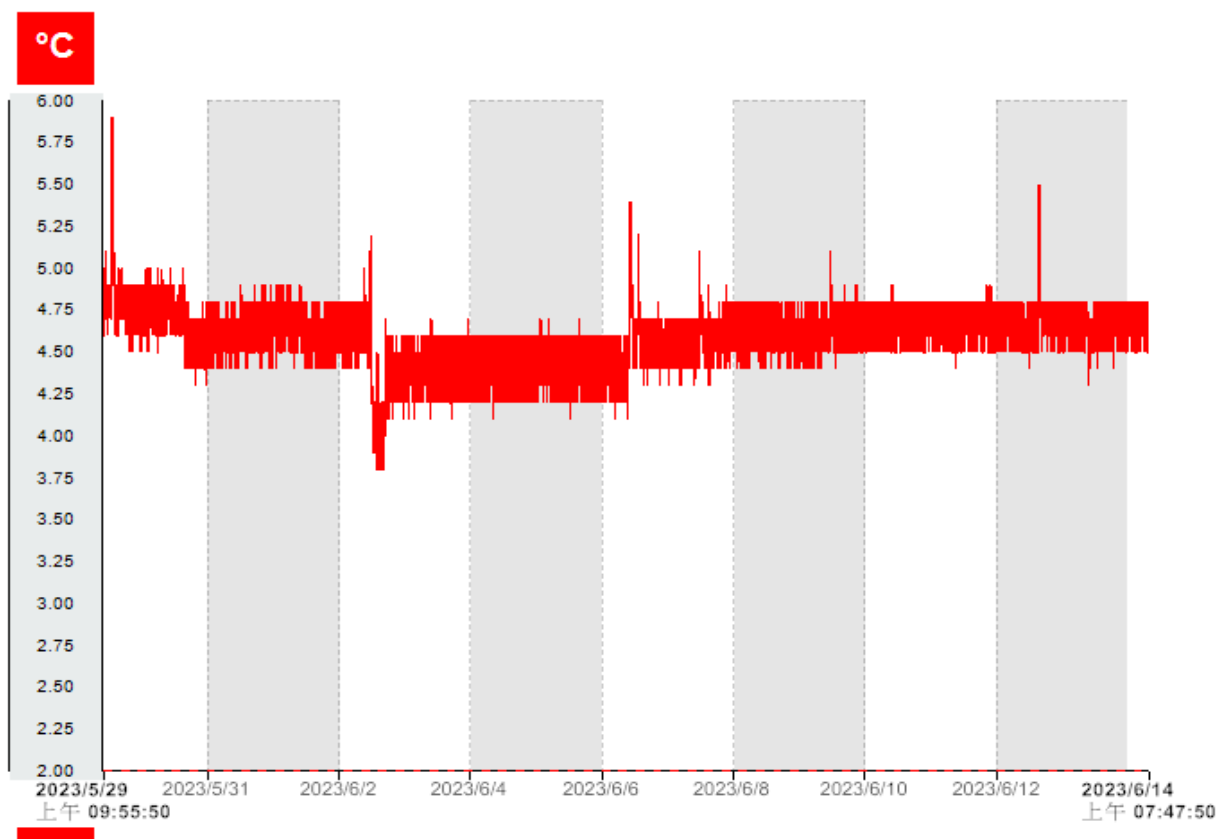

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 1D220605896; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 14, Jun 2023 ~ 14, Jun 2023



1D220605896

— v1 [°C]  
Min Max Avg Sd MKT  
4.7 5.1 4.89 0.10 4.89

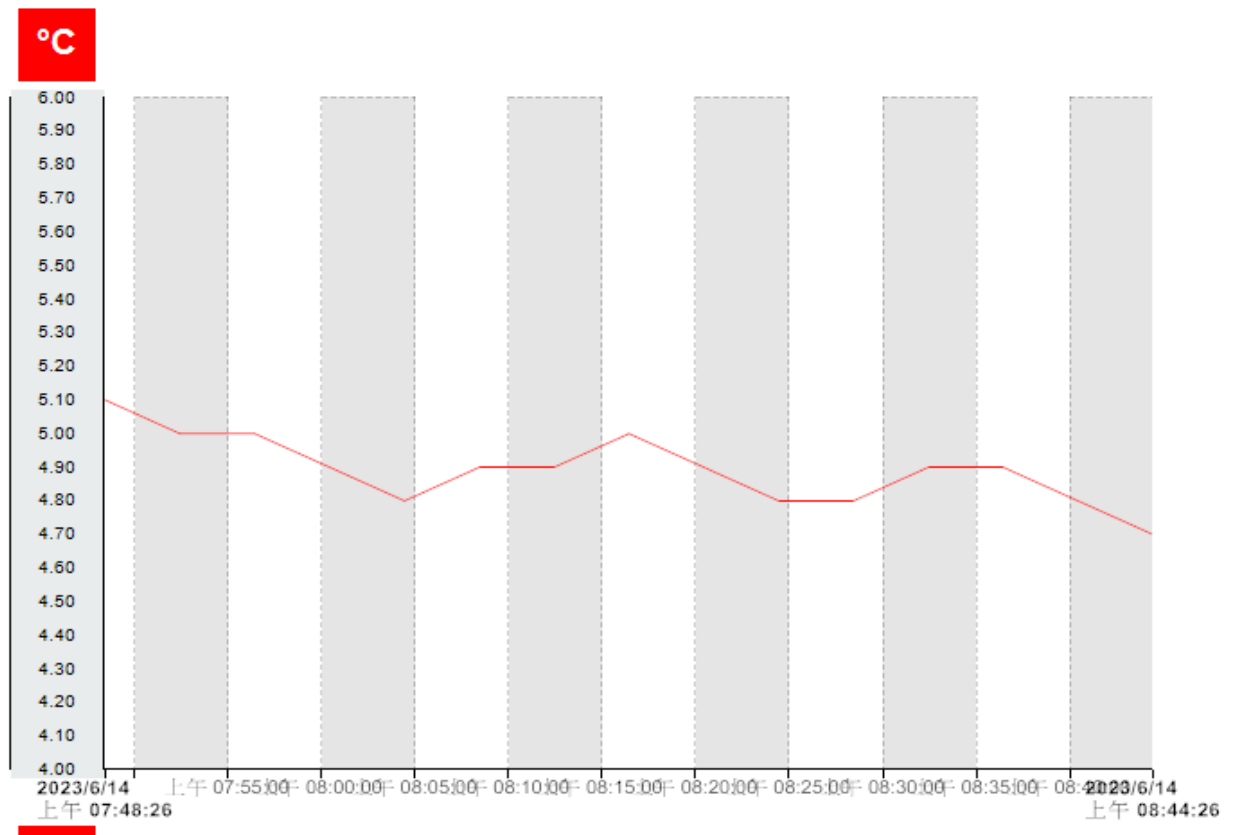

Comment: 於2023年6月14日檢查溫度記錄器2K190616069，暫以備品1D220605896代替。

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 14, Jun 2023 ~ 30, Jun 2023



**2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
3.6 5.8 4.42 0.30 4.42

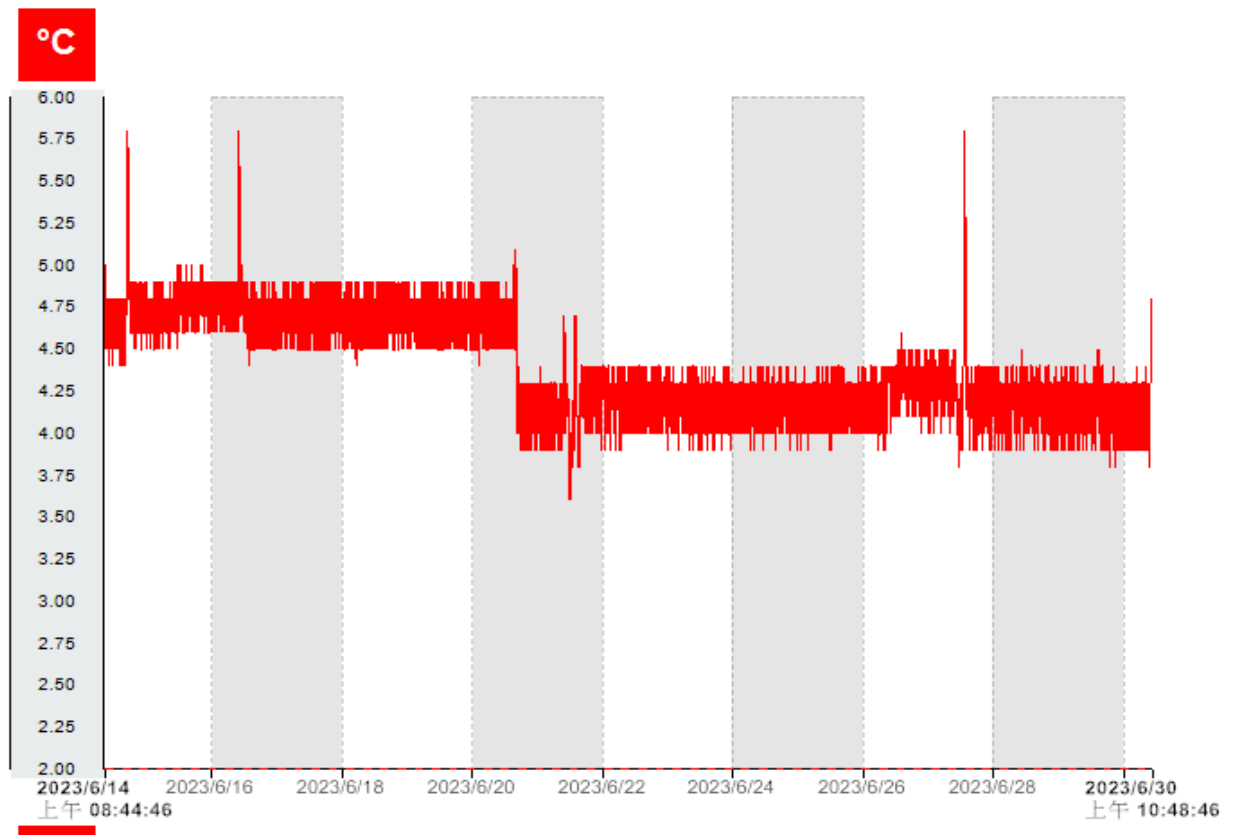

Comment:



# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K210322159; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Jun 2023 ~ 25, Jul 2023



2K210322159

— v1 [°C]  
Min Max Avg Sd MKT  
3.3 5.2 4.09 0.48 4.10

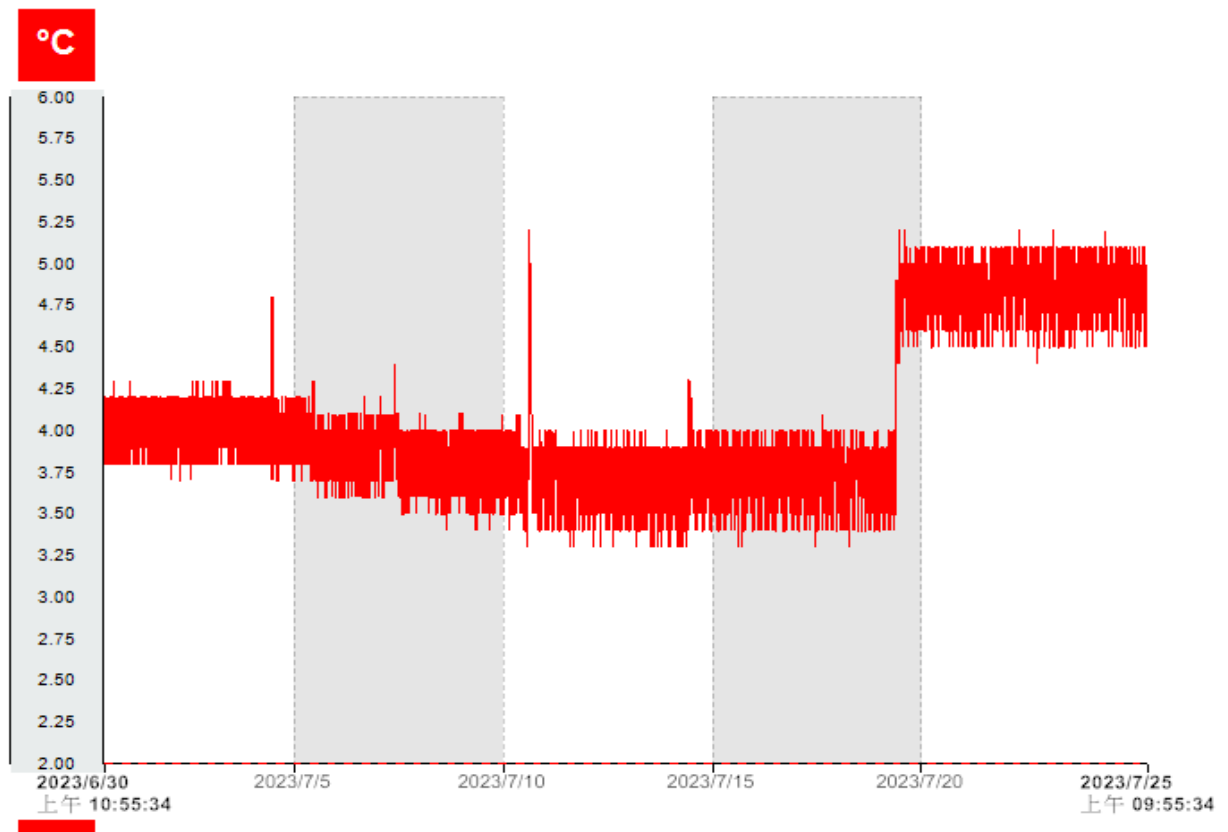

Comment: 本溫度記錄器(2K190616069)於2023年6月30日送校，期間以備品溫度記錄器(2K210322159)暫代。

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K210322159; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 25, Jul 2023 ~ 31, Jul 2023



**2K210322159**

— v1 [°C]  
Min Max Avg Sd MKT  
3.7 7.7 5.13 0.68 5.16

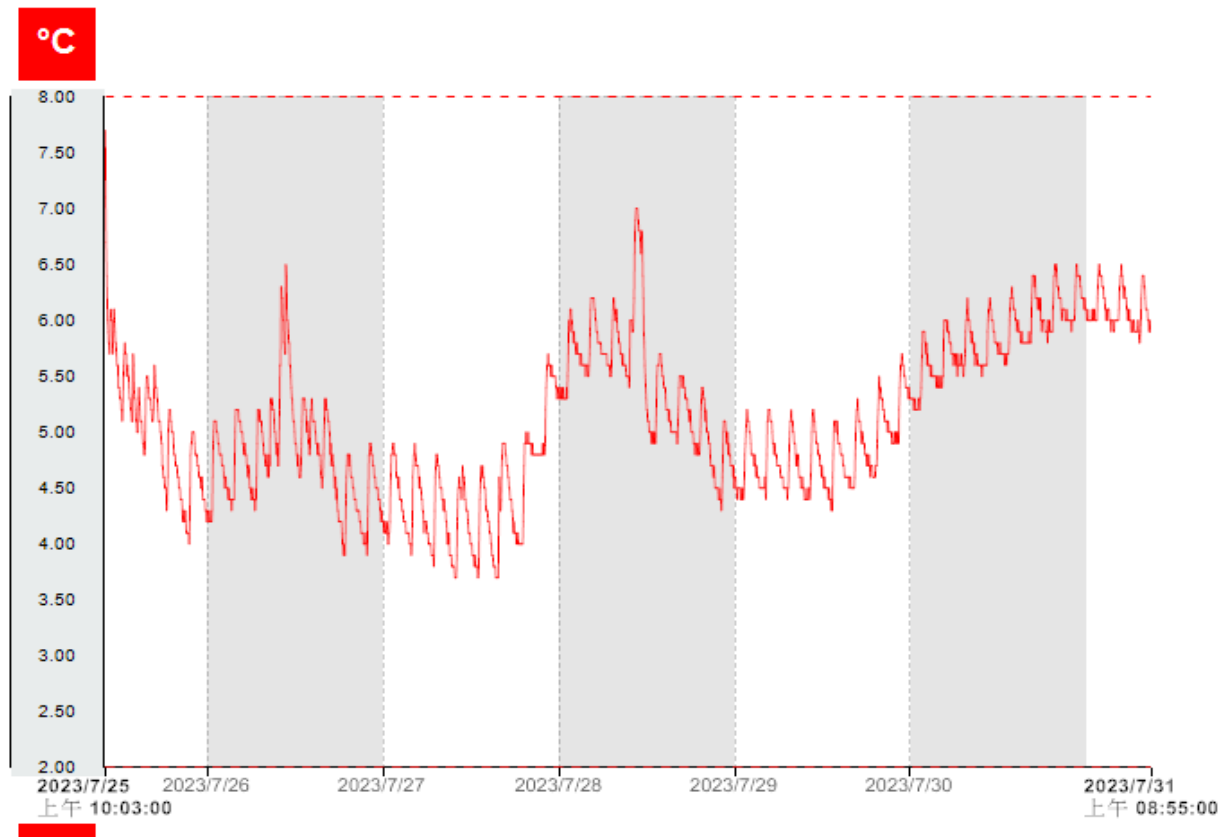

Comment: 於2023年7月25日10:00因應長庚溫控網校正，移動溫度記錄器的感溫線，調整感溫探頭後重啟。

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K210322159; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Jul 2023 ~ 01, Sep 2023



2K210322159

— v1 [°C]  
Min Max Avg Sd MKT  
3.1 6.6 4.47 0.70 4.50

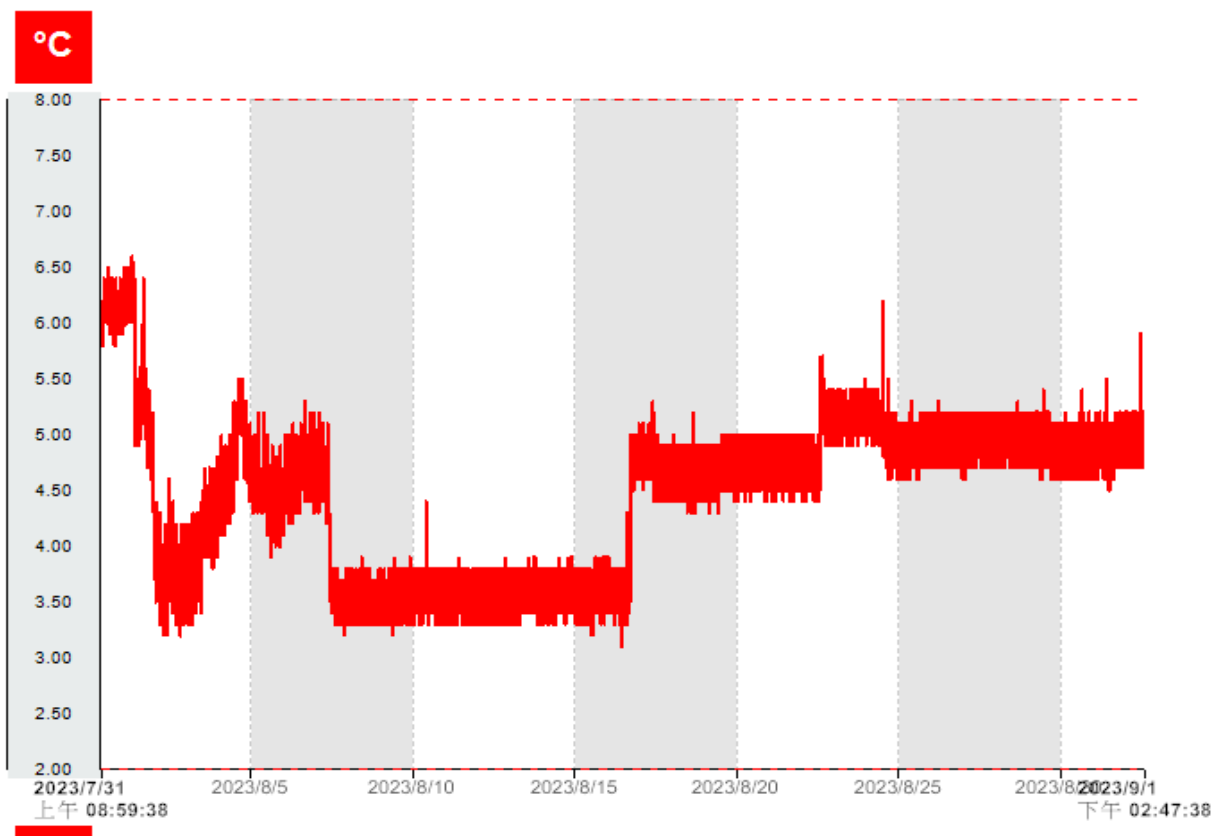



Comment:

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**THERMOMETER** : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1

**REFRIGERATOR TEMPERATURE RANGE : 2-8°C**

**DATE : 01, Sep 2023 ~ 28, Sep 2023**



# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

**PHARMACY :** B1 Medical Building , Clinical Research Pharmacy.

**REFRIGERATOR :** Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

**THERMOMETER :** Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


**REFRIGERATOR TEMPERATURE RANGE :** 2-8°C

**DATE :** 28, Sep 2023 ~ 31, Oct 2023



**2K190616069**

— v1 [°C]  
Min Max Avg Sd MKT  
3.2 5.5 4.66 0.32 4.66

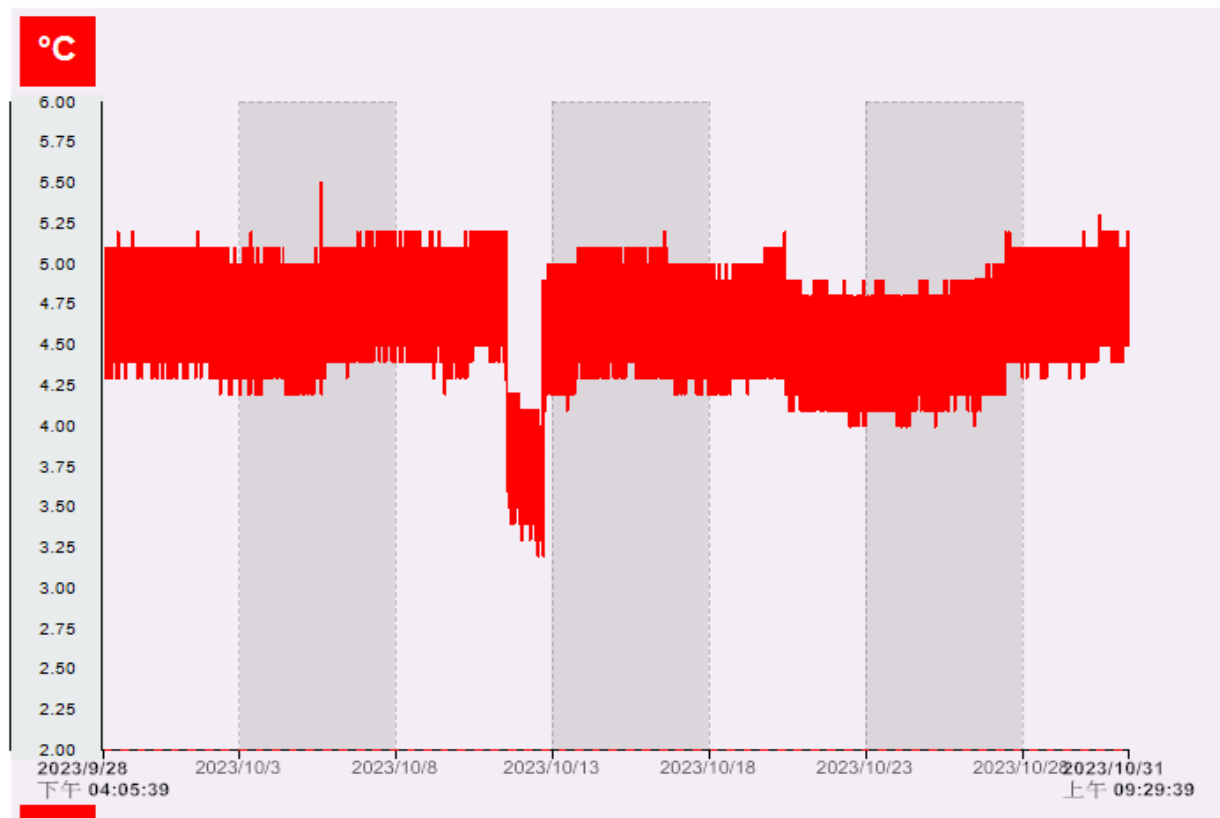

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31, Oct 2023 ~ 30, Nov 2023



2K190616069

— v1 [°C]  
Min Max Avg Sd MKT  
3.8 5.8 4.61 0.29 4.62

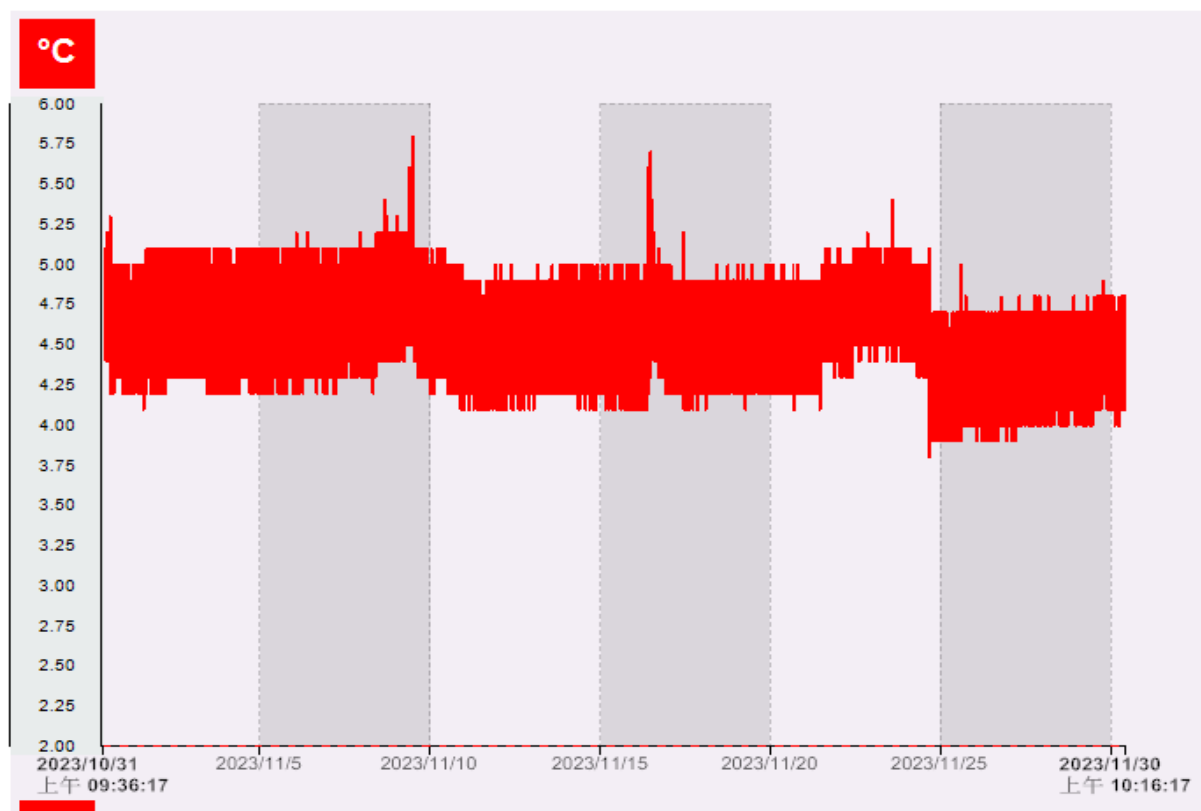

Comment:

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No. : 1207 0022

THERMOMETER : Manufacturer : KIMO; Model No.: KTT-220-O; Serial No.: 2K190616069; Channel No.: 1


REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 30, Nov 2023 ~ 29, Dec 2023



2K190616069

— v1 [°C]  
Min Max Avg Sd MKT  
3.7 5.6 4.44 0.29 4.44

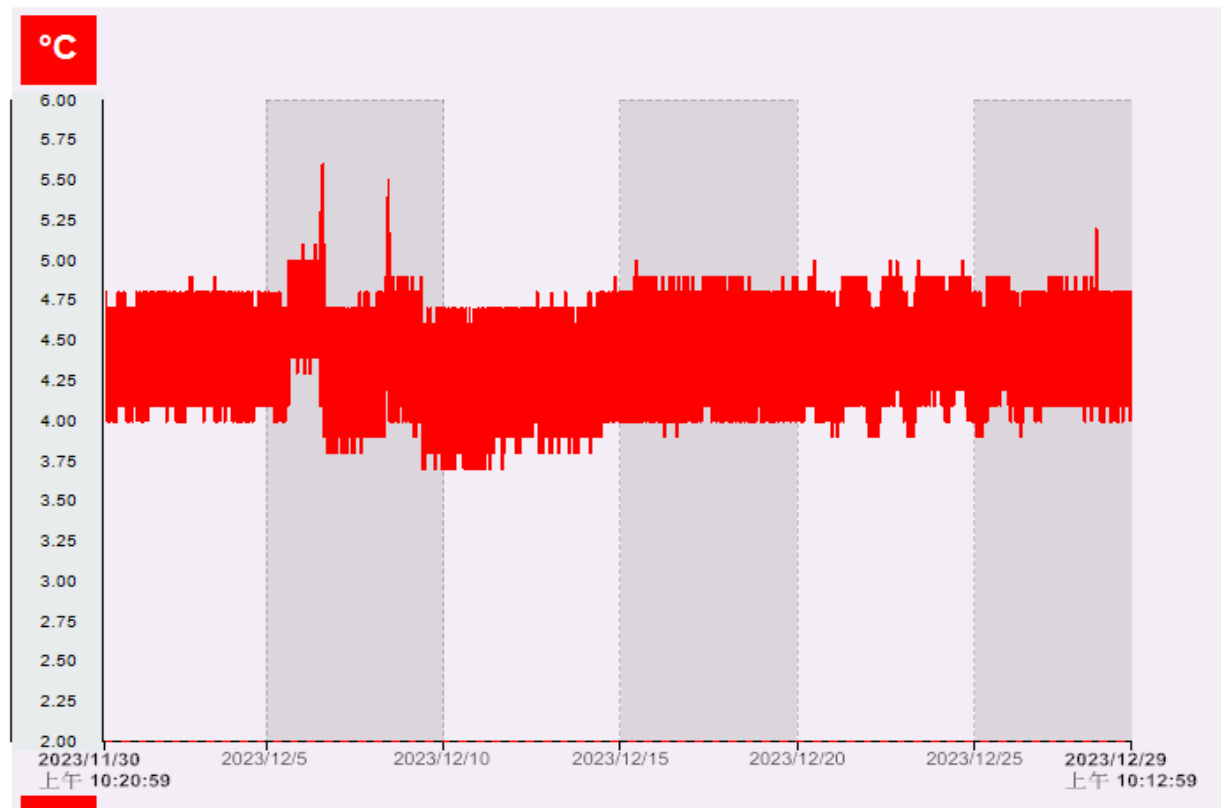

Comment: