

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 29, Dec 2023 ~ 31, Jan 2024

Instrument name: Testo 176T2		2024/2/1 上午 10:40:53			Page	1/1
Starttime: 2023/12/29 上午 10:59:13		Minimum	Maximum	Mean value	Limit values	
End time: 2024/1/31 上午 08:59:13	40505446 [°C]	-74.96	-72.50	-73.792	-80.0/-80.0	
Measurement channels: 1						
Measured values: 791						
SN 40505446						

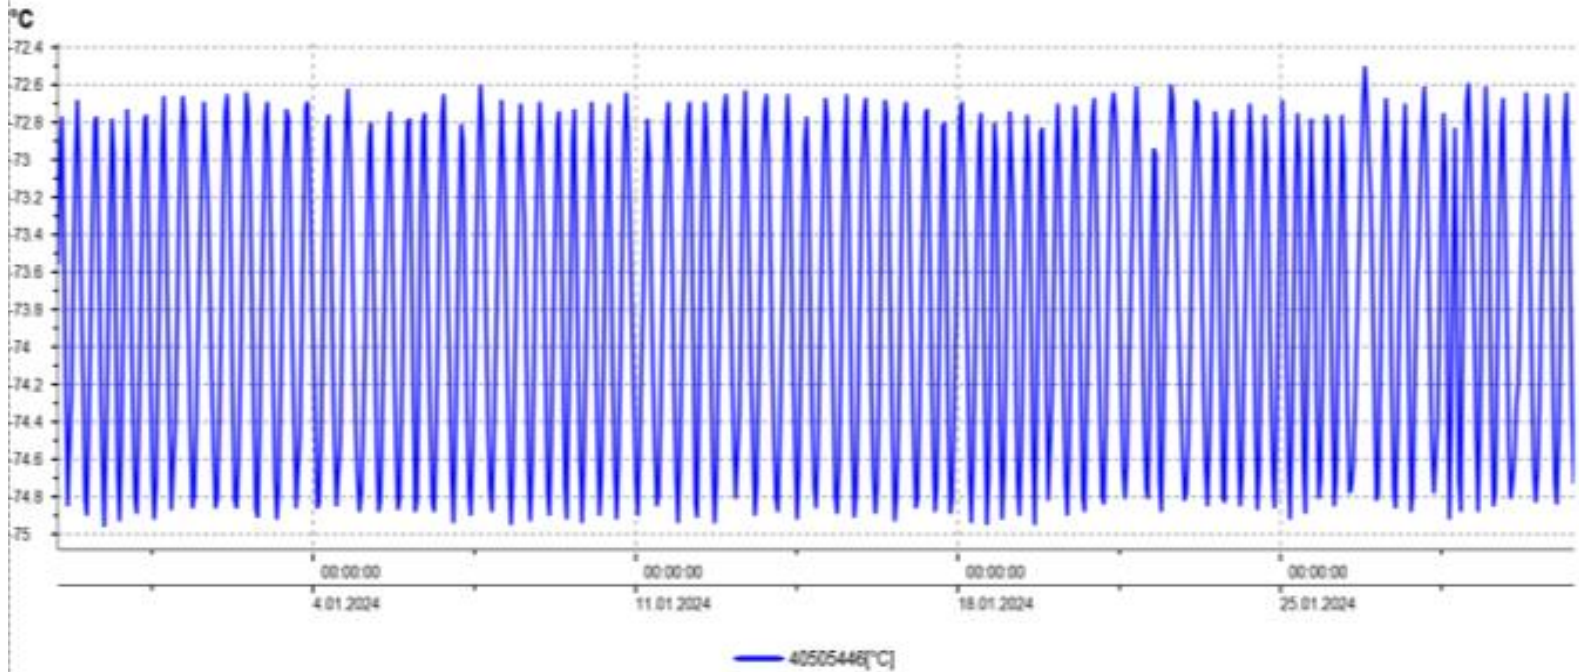

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31, Jan 2024 ~ 28, Feb 2024

Instrument name: Testo 176T2		2024/2/28 下午 03:41:00			Page 1/1
Starttime: 2024/1/31 上午 09:07:36		Minimum	Maximum	Mean value	Limit values
End time: 2024/2/28 下午 03:07:36	40505446 [°C]	-74.91	-72.48	-73.713	-80.0/-60.0
Measurement channels: 1					
Measured values: 679					
SN 40505446					

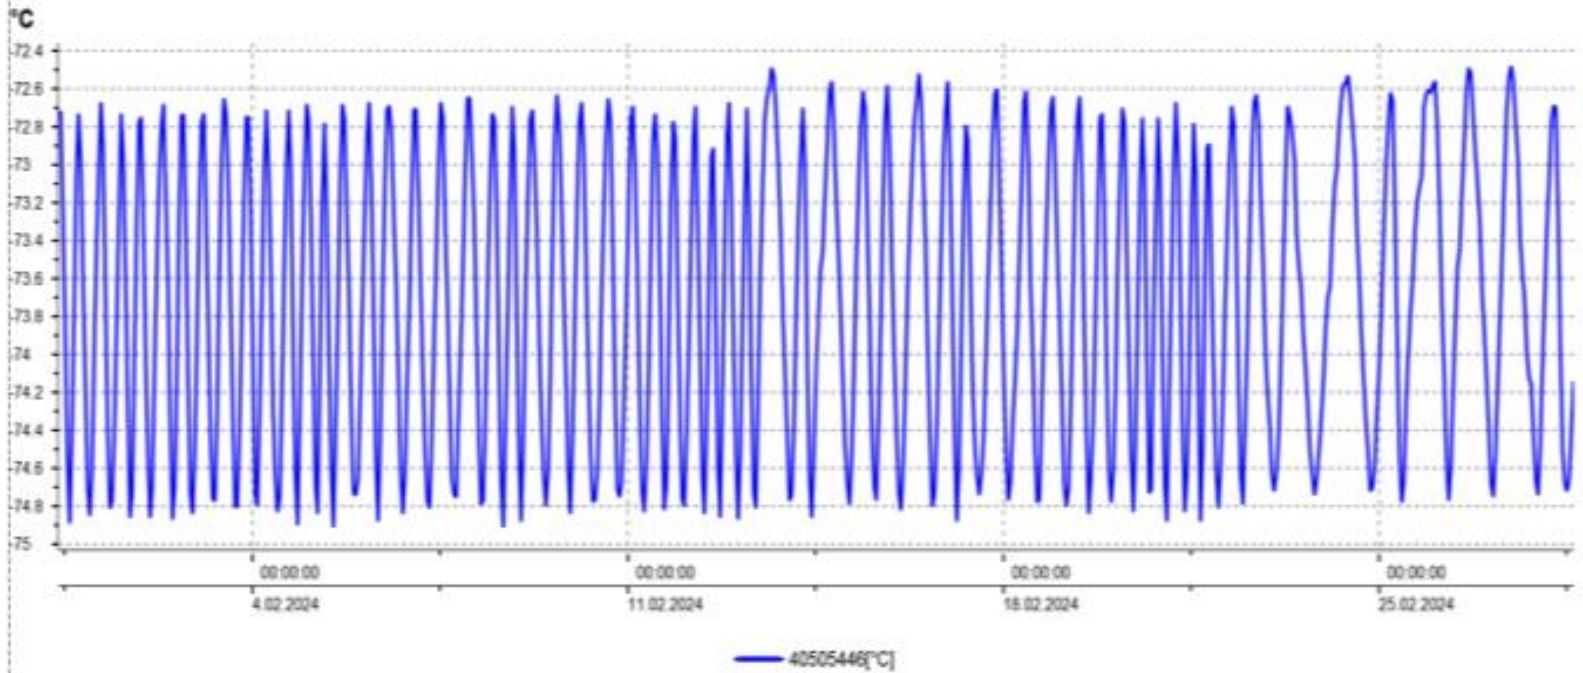

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 28, Feb 2024 ~ 1, Apr 2024

Instrument name: Testo 176T2		2024/4/2 上午 09:17:51			Page	1/1
Starttime: 2024/2/28 下午 03:13:59		Minimum	Maximum	Mean value	Limit values	
Endtime: 2024/4/1 上午 08:13:59	40505446 [°C]	-74.84	-72.42	-73.686	-80.0/-80.0	
Measurement channels: 1						
Measured values: 786						
SN 40505446						

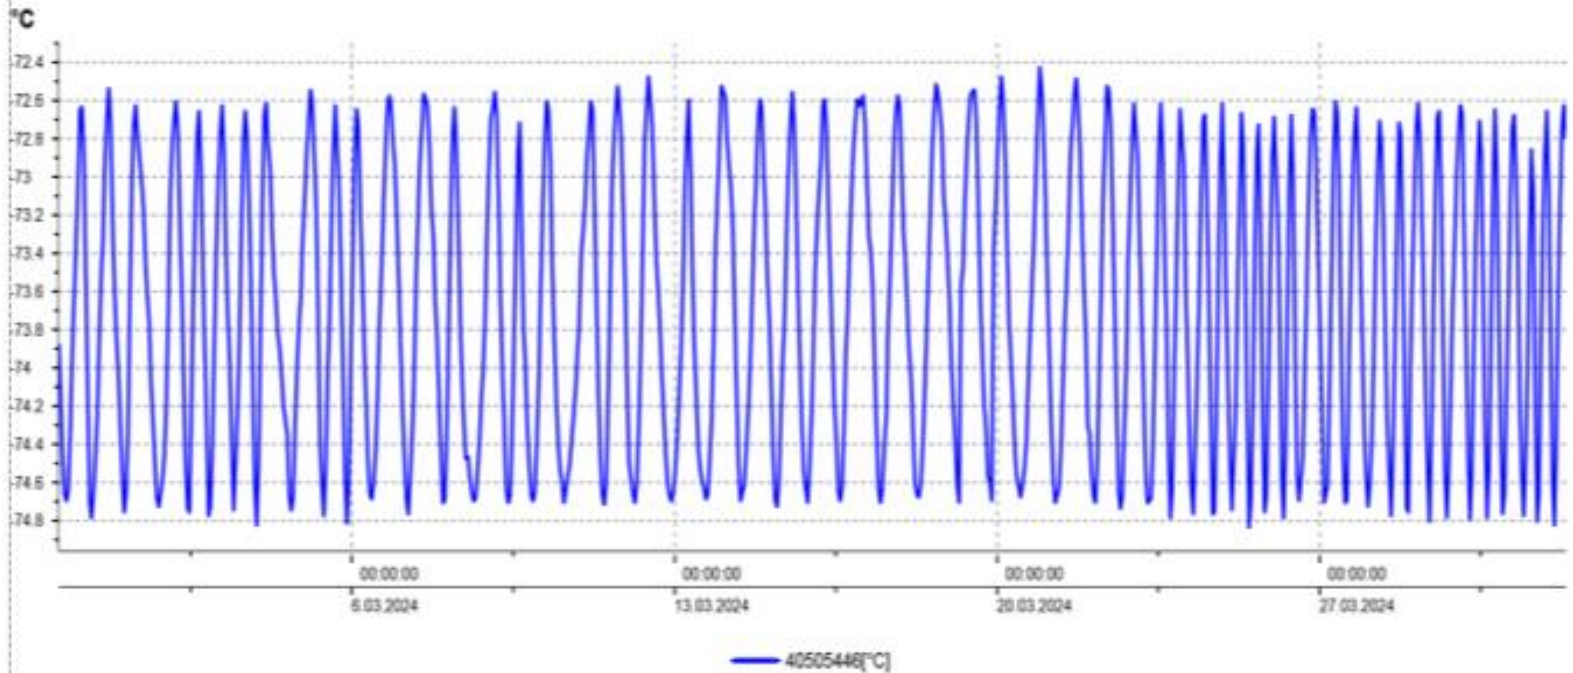

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 1, Apr 2024 ~ 29, Apr 2024

Instrument name: Testo 176T2		2024/4/29 上午 11:15:28			Page	1/1
Starttime: 2024/4/1 上午 08:37:09		Minimum	Maximum	Mean value	Limit values	
End time: 2024/4/29 上午 09:37:09	40505446 [°C]	-74.89	-72.53	-73.664	-80.0/-80.0	
Measurement channels: 1						
Measured values: 674						
SN 40505446						

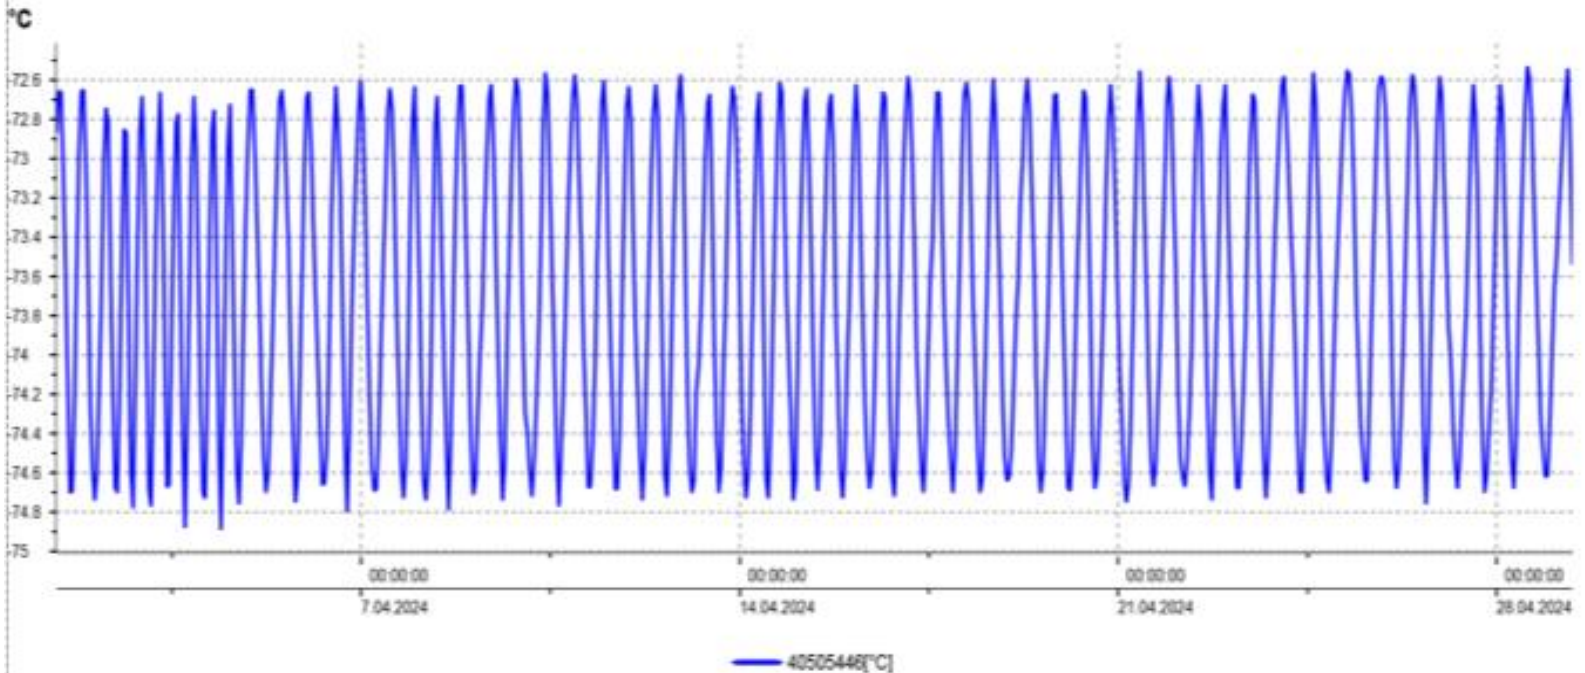

Comment: