

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 29, Dec 2023 ~ 31, Jan 2024



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.4 -18.9 -19.77 0.57 -19.75

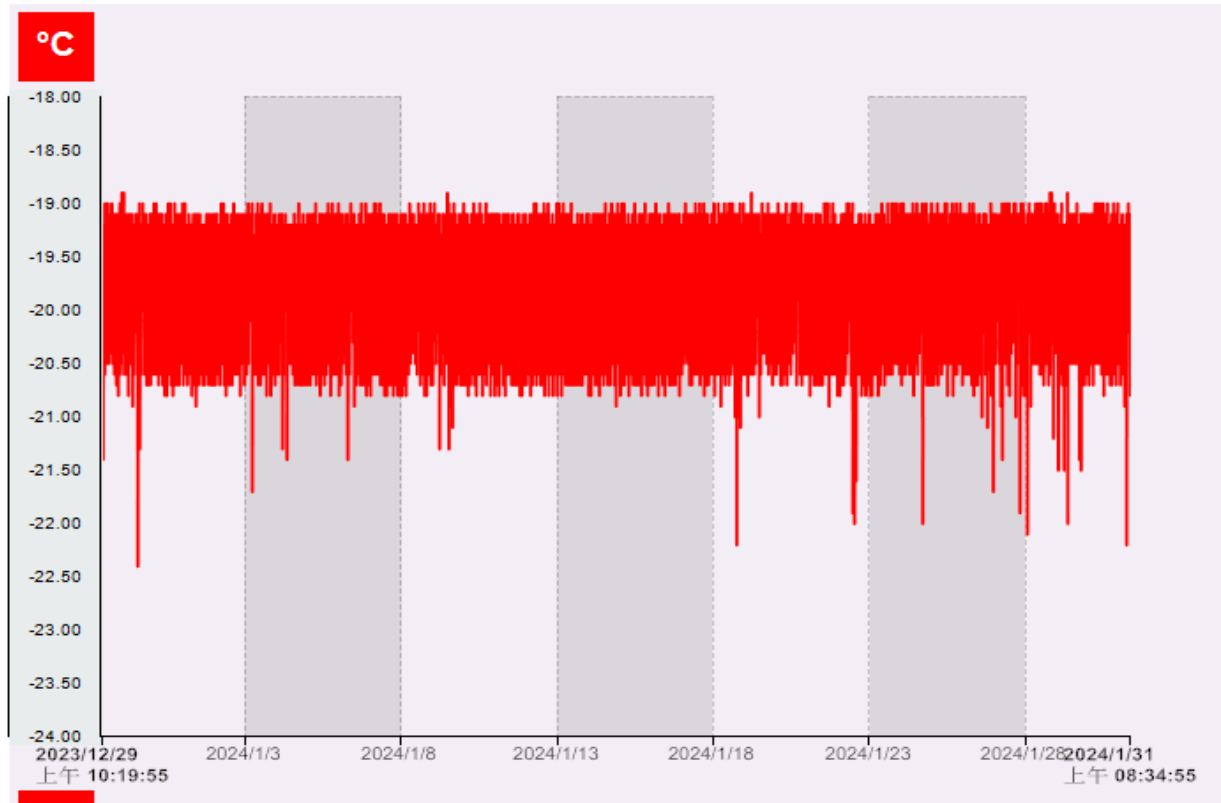

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31, Jan 2024 ~ 28, Feb 2024



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.6 -18.9 -19.80 0.64 -19.77

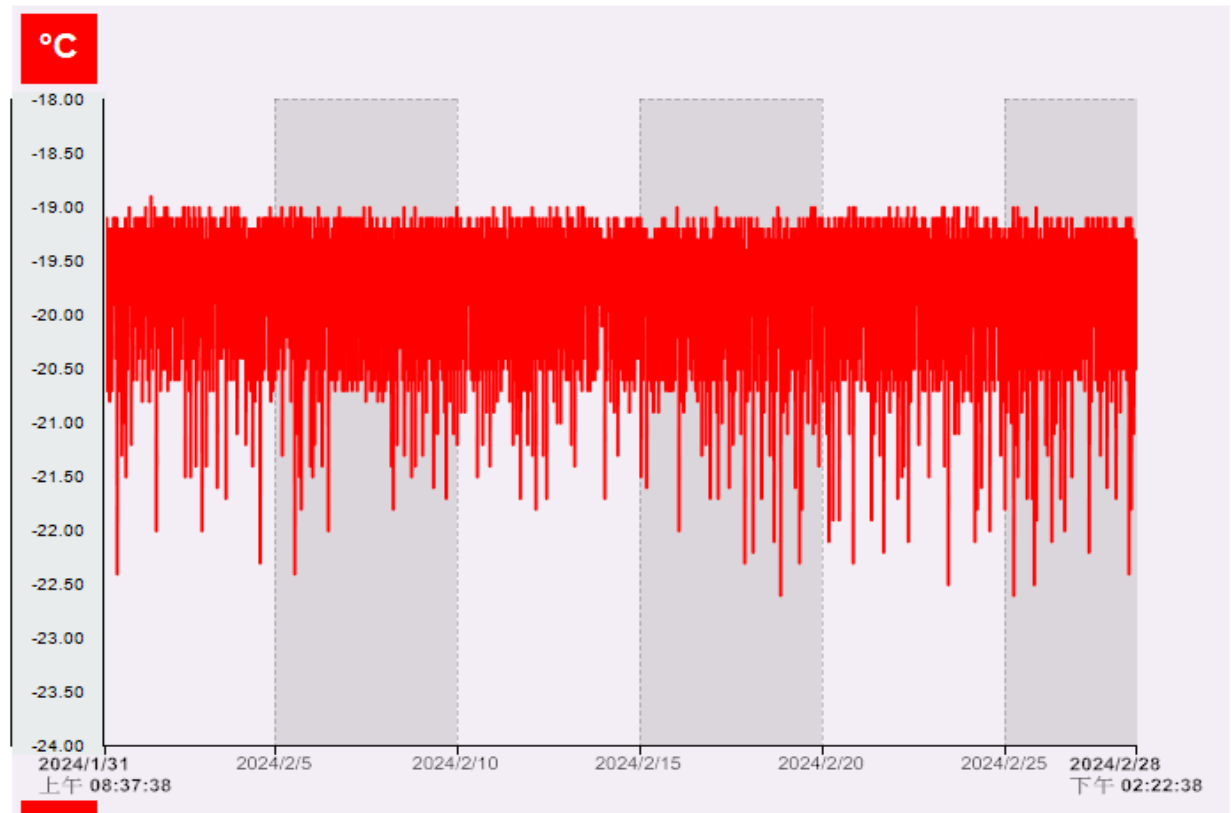

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 28, Feb 2024 ~ 1, Apr 2024



2K210923833

— v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.9 -18.4 -19.88 0.69 -19.85

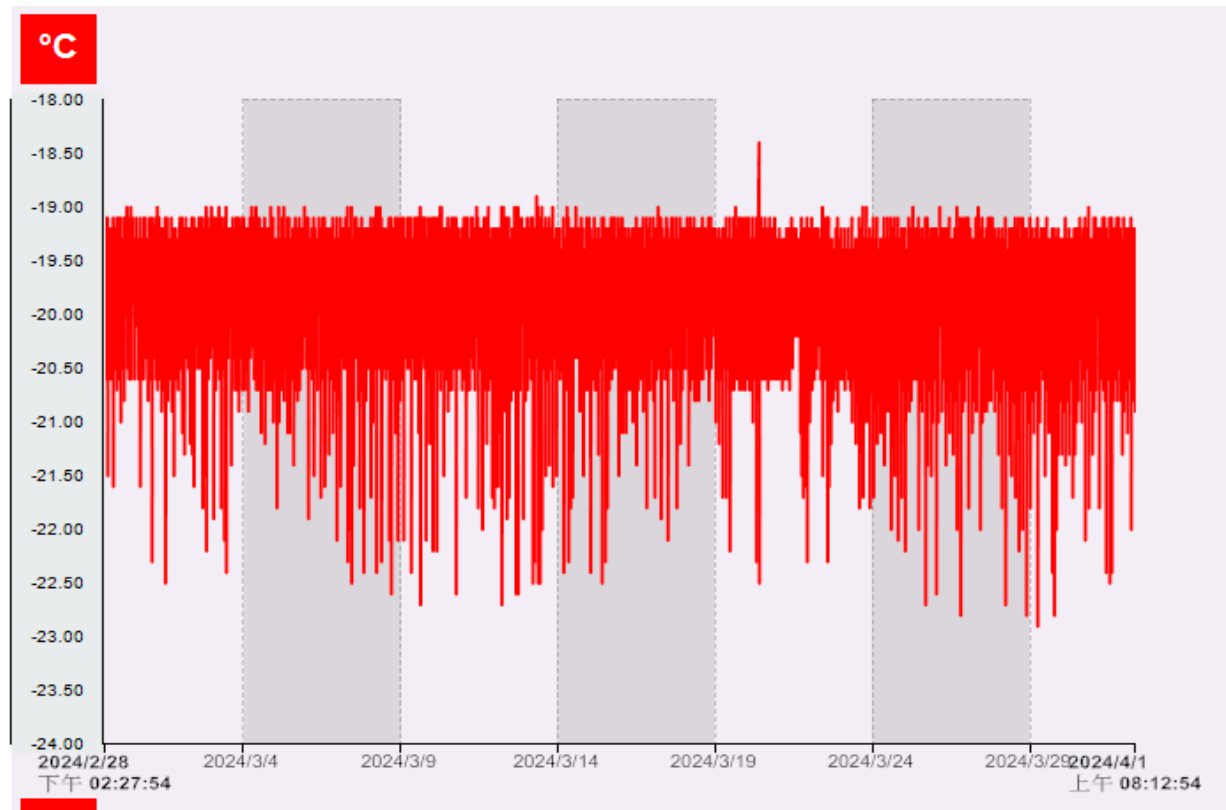

Comment:本冷凍櫃（冷凍2上層）於2024年3月21日08:49開始儲存藥品，並於2024年3月22日17:01將藥品移回冷凍2下層。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 1, Apr 2024 ~ 29, Apr 2024



2K210923833

v1 2K210923833 [°C]
Min Max Avg Sd MKT
-22.9 -19.0 -19.97 0.73 -19.93

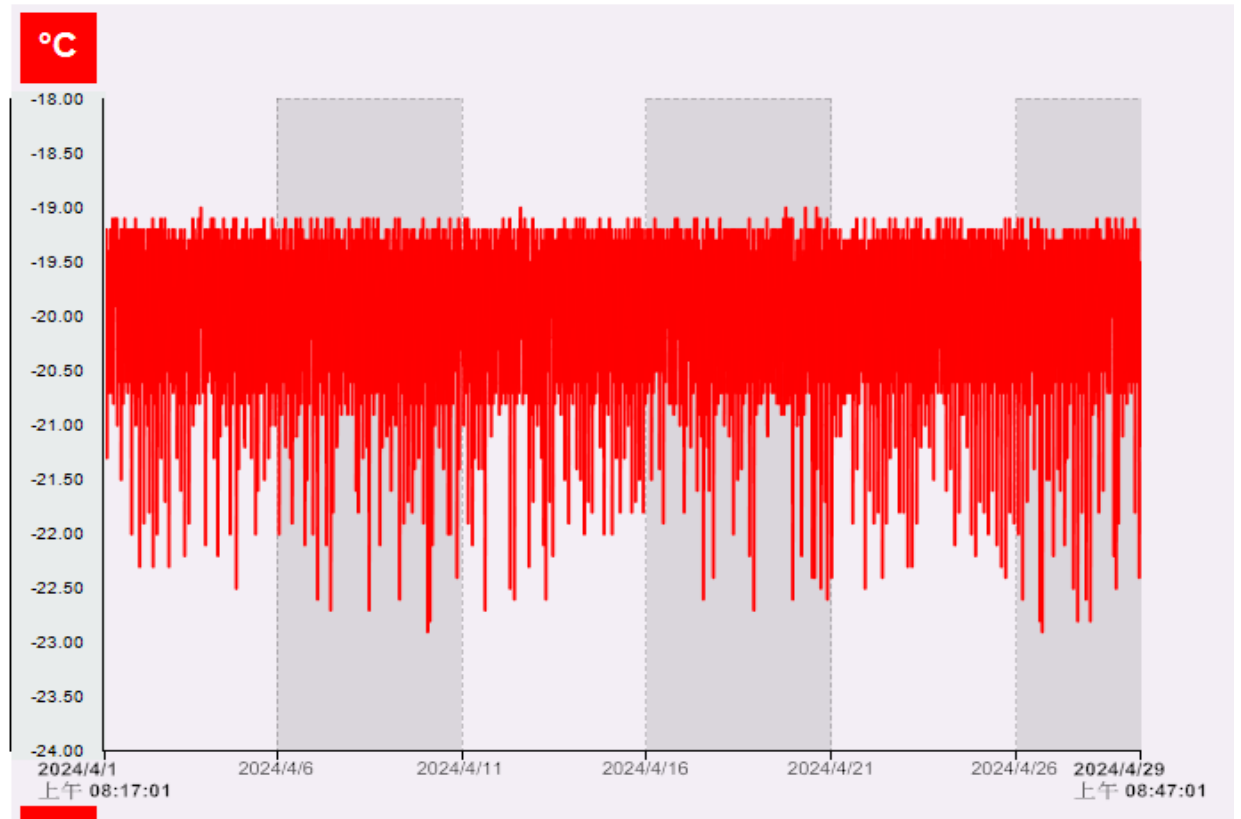

Comment: