

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1

FREEZER TEMPERATURE RANGE : 2-8°C


DATE : **29, Dec 2023 ~ 29, Dec 2023**

統計圖表 > log資料查詢

組別 : 臨床試驗藥局 ; 設備 : 臨床試驗藥局 冷藏1 ; 可容許上下限值 : 2.5 ~ 7.5

最小值 : 3.7 ; 最大值 : 4.2 ; 平均值 : 3.97

時間範圍 : 2023-12-29 10:00:00 ~ 2023-12-29 10:30:00 ; 取樣率 : 1 : 1

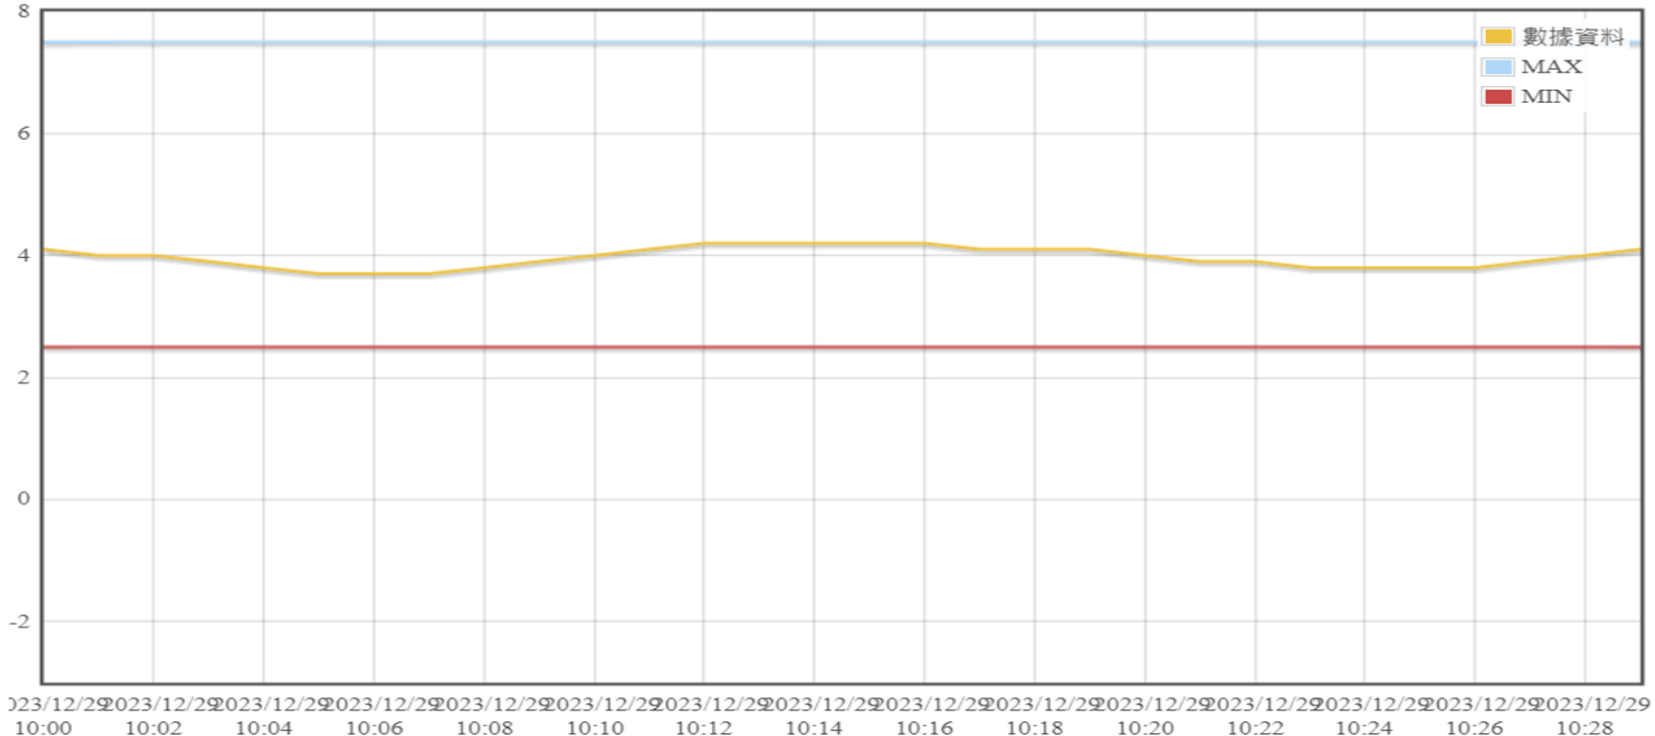

Comment:溫度記錄器於2023年12月29日10:00~10:28故障未測到資料，故以長庚溫控網溫度記錄佐證。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1

FREEZER TEMPERATURE RANGE : 2-8°C


DATE : 29, Dec 2023 ~ 31, Jan 2024



2K210923834

— v1 [°C]

| Min | Max | Avg | Sd | MKT |
|-----|-----|------|------|------|
| 3.5 | 5.0 | 4.20 | 0.32 | 4.21 |

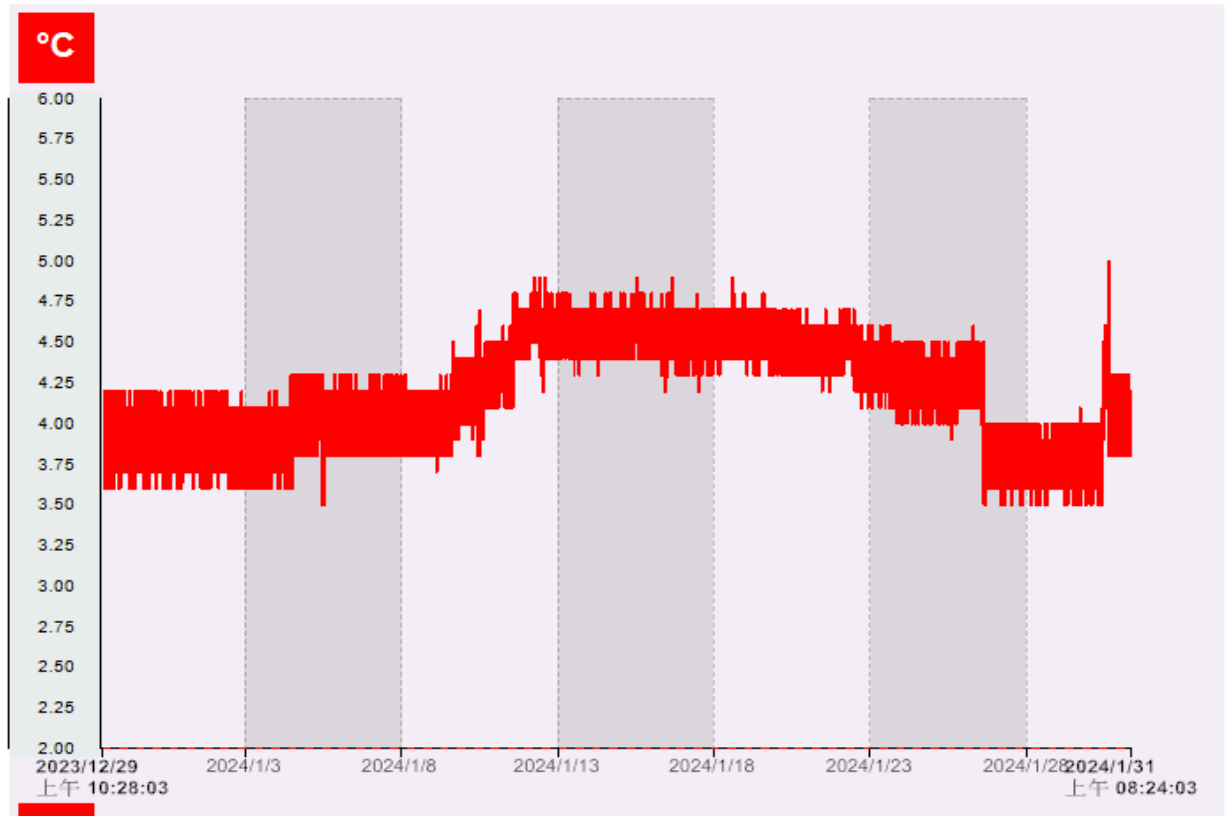

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 31, Jan 2024 ~ 28, Feb 2024



2K210923834

| | | | | |
|-----------|-----|------|------|------|
| — v1 [°C] | | | | |
| Min | Max | Avg | Sd | MKT |
| 3.8 | 5.3 | 4.33 | 0.18 | 4.33 |

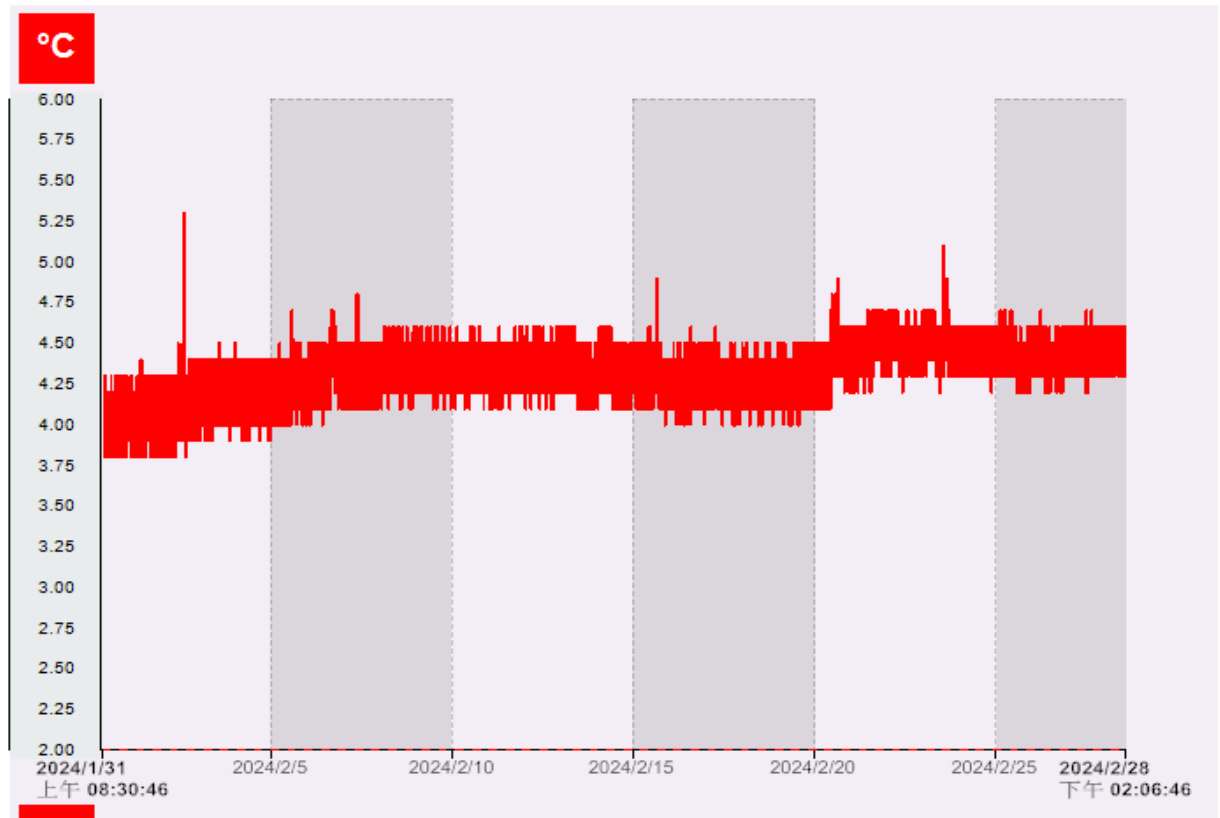

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 28, Feb 2024 ~ 5, Mar 2024



2K210923834

| v1 [°C] | | | | |
|---------|-----|------|------|------|
| Min | Max | Avg | Sd | MKT |
| 4.1 | 4.8 | 4.40 | 0.12 | 4.41 |

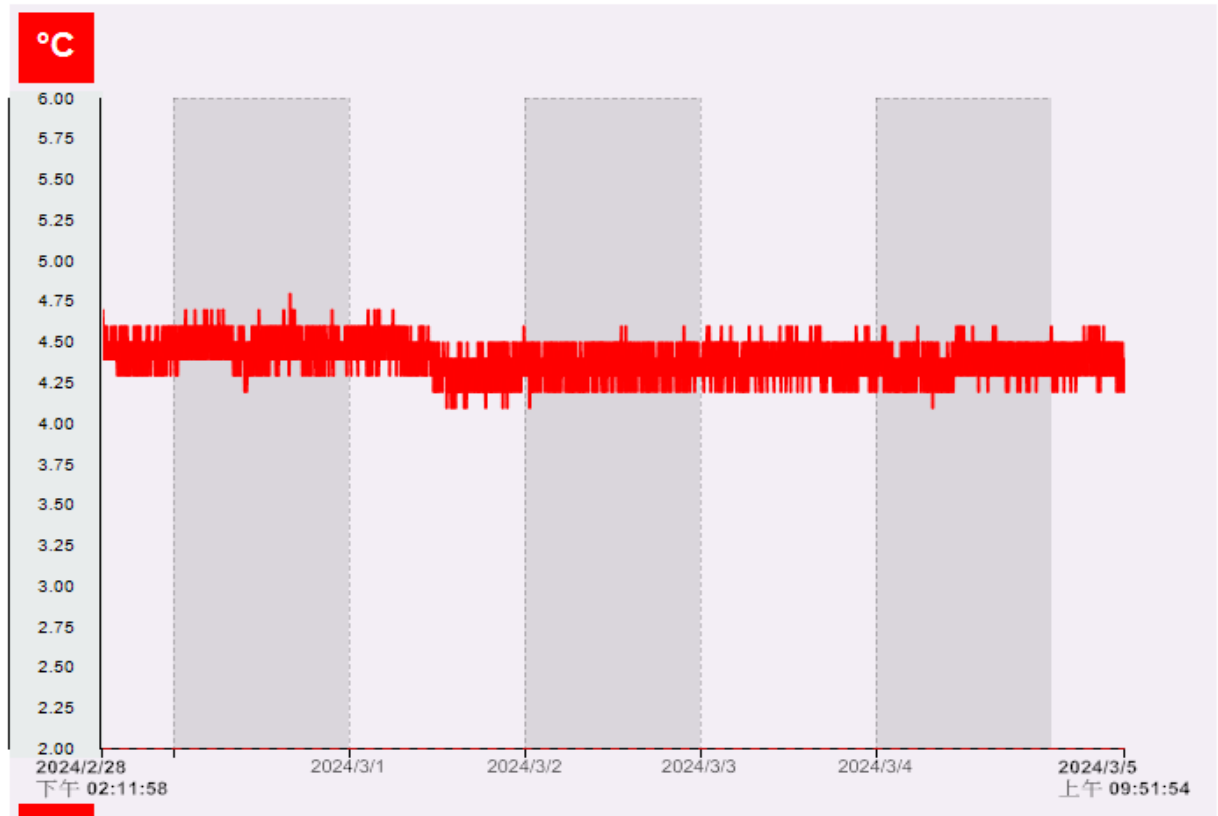

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1

FREEZER TEMPERATURE RANGE : 2-8°C


DATE : 5, Mar 2024 ~ 5, Mar 2024

統計圖表 > log資料查詢

組別 : 臨床試驗藥局 ; 設備 : 臨床試驗藥局 冷藏1 ; 可容許上下限值 : 2.5 ~ 7.5

最小值 : 4.0 ; 最大值 : 4.6 ; 平均值 : 4.27

時間範圍 : 2024-03-05 09:45:00 ~ 2024-03-05 17:00:00 ; 取樣率 : 1 : 1

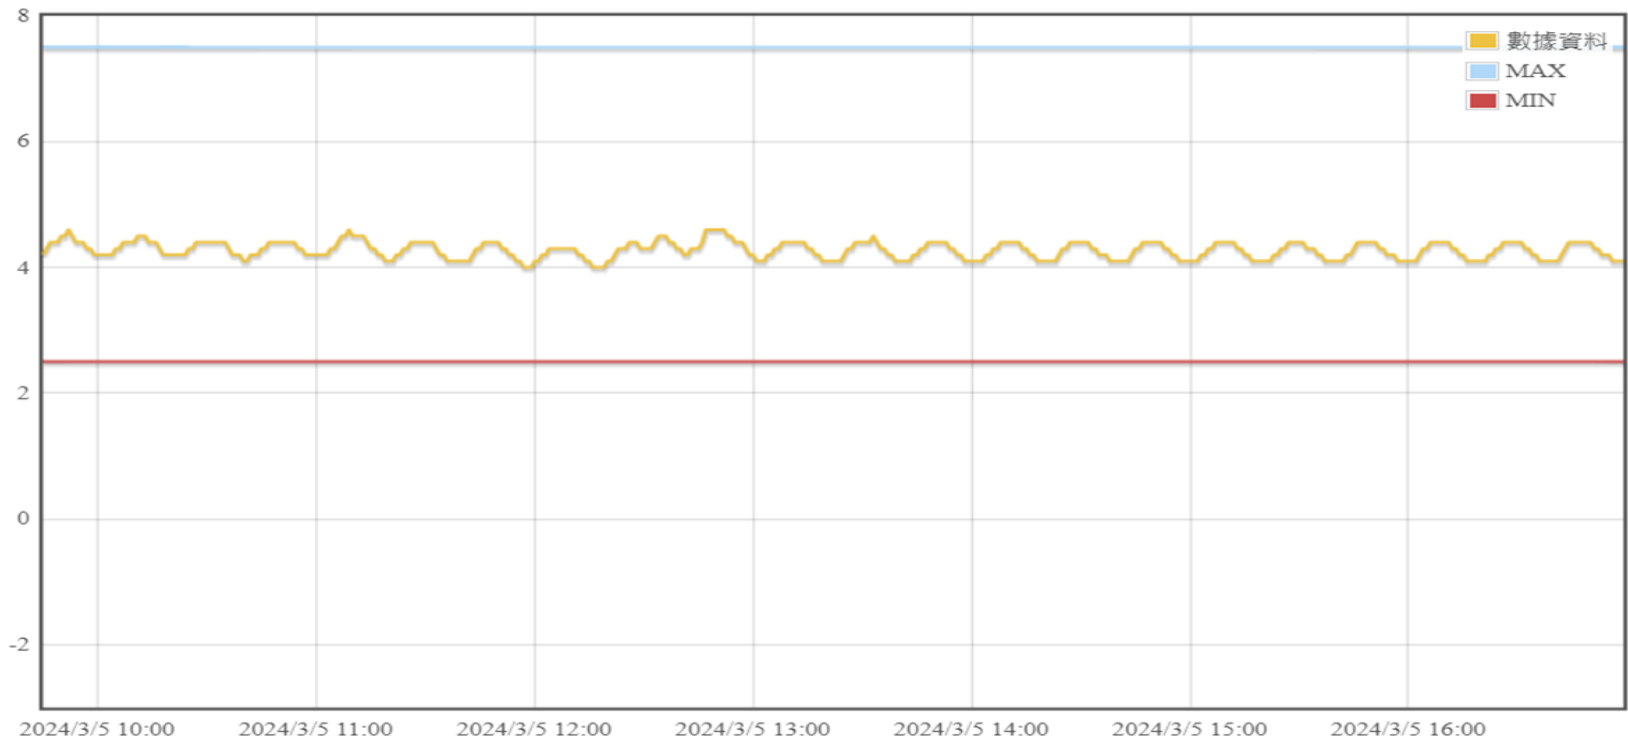

Comment:溫度記錄器於2024年3月5日09:51~16:46故障未測到資料，故以長庚溫控網溫度記錄佐證。

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 5, Mar 2024 ~ 1, Apr 2024



2K210923834

| | | | | |
|-----------|-----|------|------|------|
| — v1 [°C] | | | | |
| Min | Max | Avg | Sd | MKT |
| 3.9 | 5.6 | 4.33 | 0.15 | 4.33 |

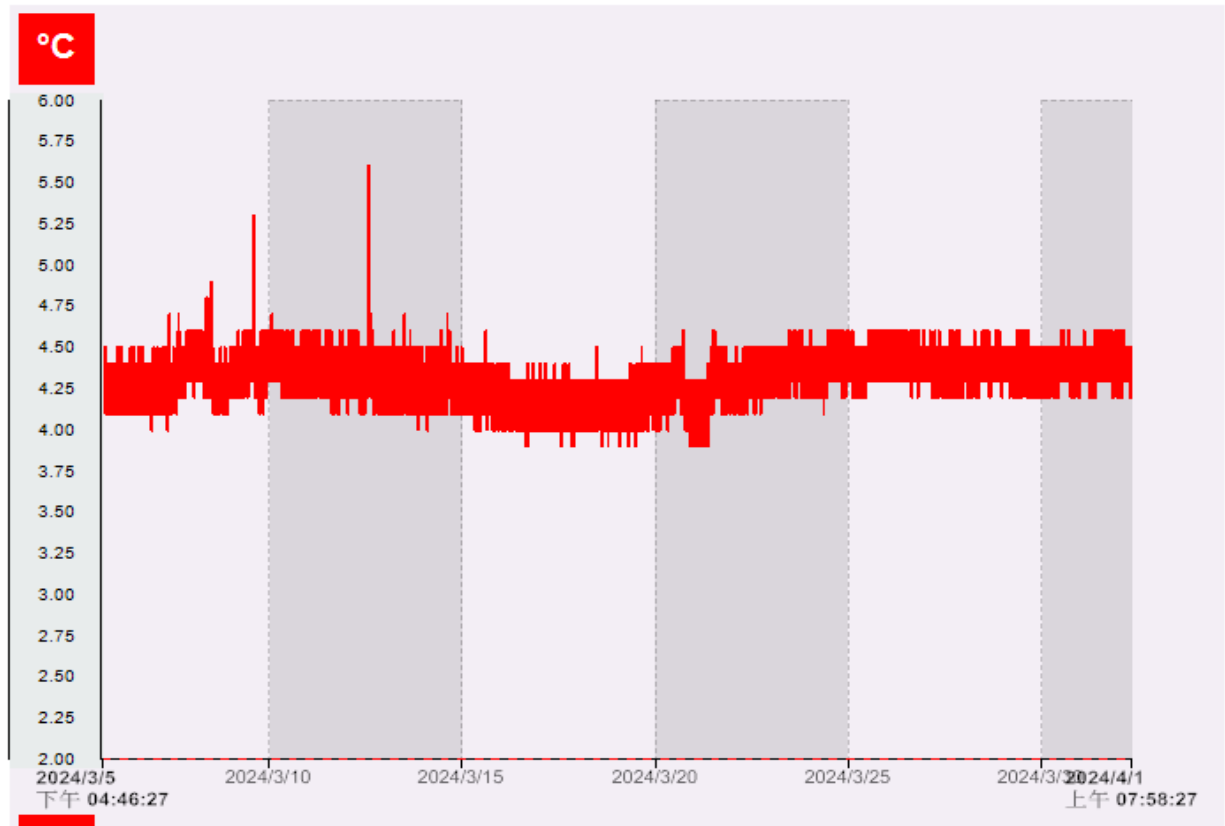

Comment:

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 12110043

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-220-O; Serial No.: 2K210923834; Channel No.: 1


FREEZER TEMPERATURE RANGE : 2-8°C

DATE : 1, Apr 2024 ~ 29, Apr 2024



2K210923834

| | | | | |
|-----------|-----|------|------|------|
| — v1 [°C] | | | | |
| Min | Max | Avg | Sd | MKT |
| 3.8 | 4.8 | 4.21 | 0.20 | 4.21 |

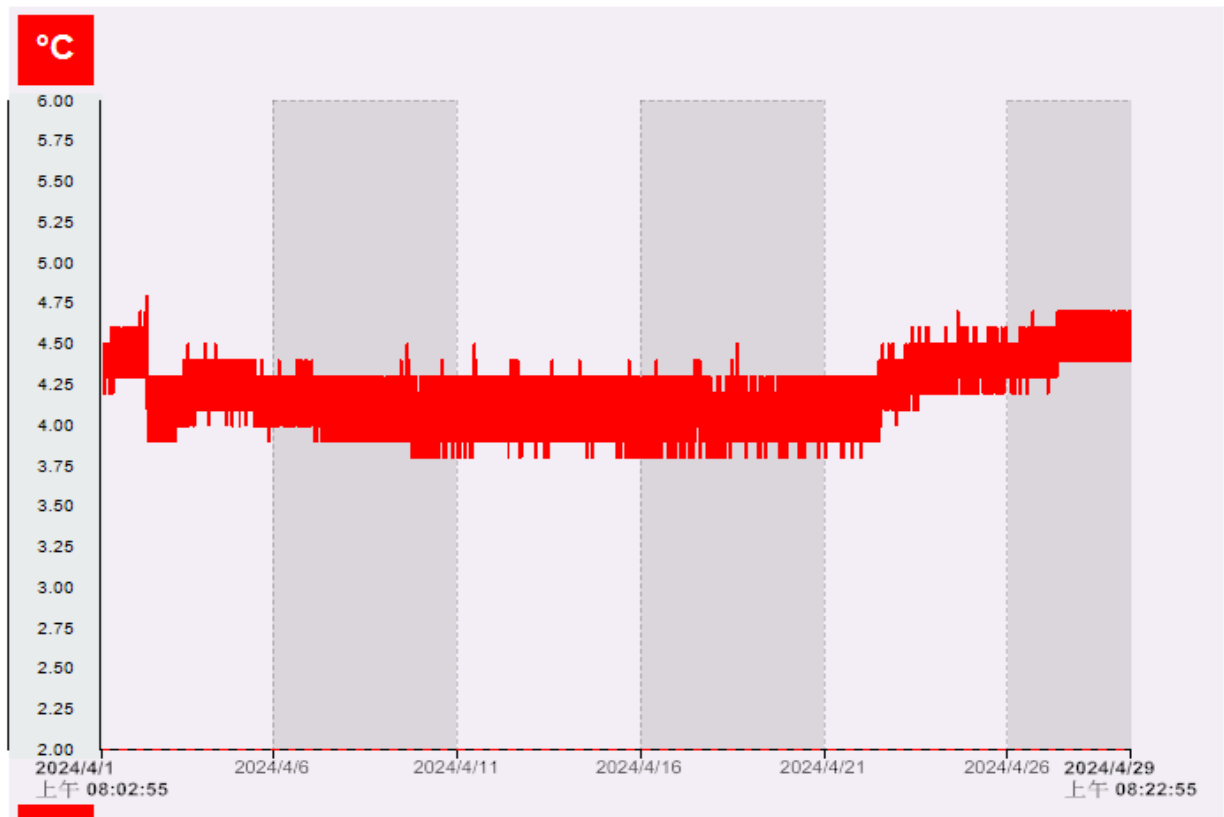

Comment: