

長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building , Clinical Research Pharmacy.


REFRIGERATOR : Manufacturer : VESTFROST SOLUTIONS ; Model No. : VT-78 ; Serial No. : 20151589264

THERMOMETER : Manufacturer : TESTO ; Model No.: 176-T2 ; Serial No. : 40505446; Channel No. : 1

REFRIGERATOR TEMPERATURE RANGE : -70± 10 °C

DATE : 31 Dec 2024 ~ 24 Jan 2025

Instrument name: Testo 176T2		2025/1/24 上午 09:51:38			Page 1/1
Start time: 2024/12/31 上午 11:23:28		Minimum	Maximum	Mean value	Limit values
End time: 2025/1/24 上午 09:23:28	40505446 [°C]	-73.20	-70.98	-72.070	-80.0/-60.0
Measurement channels: 1					
Measured values: 575					
SN40505446					

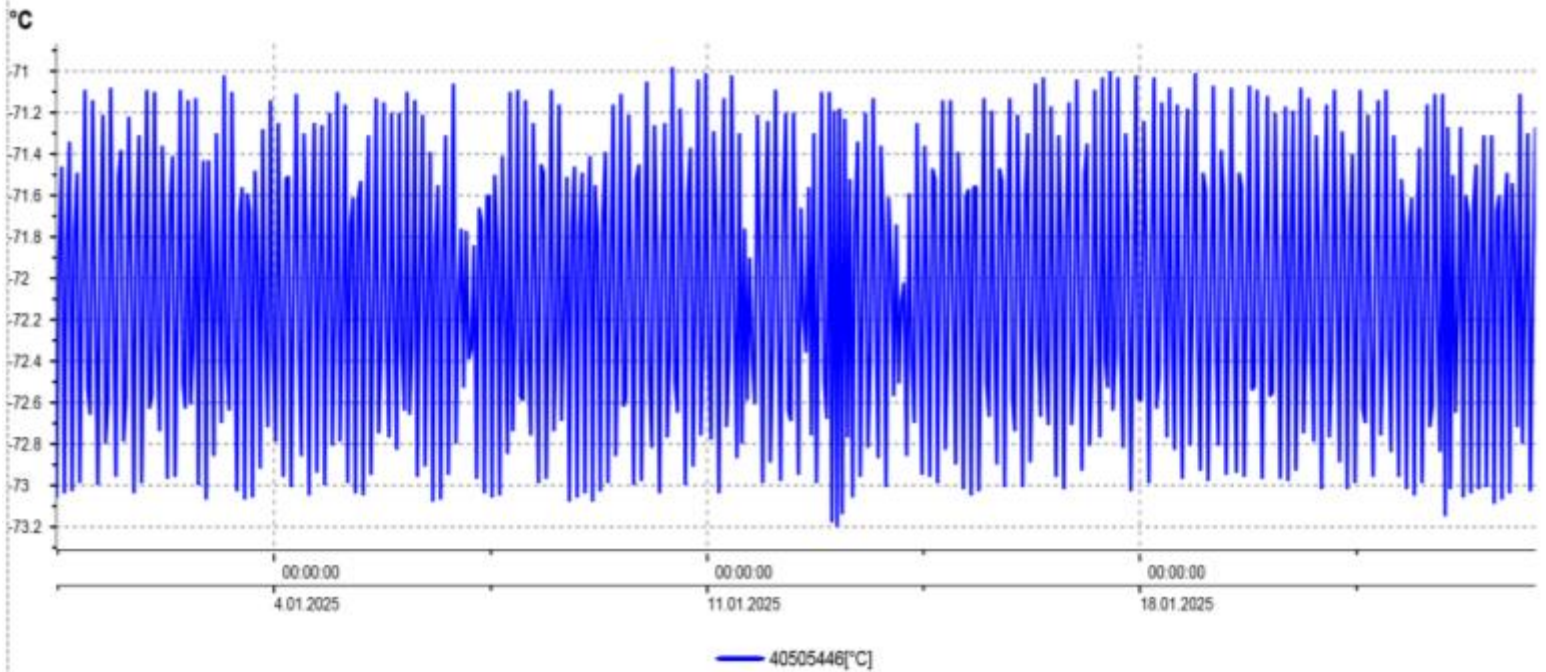

Comment: