

# 長庚紀念醫院—林口院區 藥品保存溫度記錄表

PHARMACY : B1 Medical Building, Clinical Research Pharmacy

FREEZER : Manufacturer; SANYO; Model No.: MDF-U537D; Serial No.: 10040043; Chamber : top

THERMOMETER : KIMO; Model No.: KTT-220-O; Serial No.: 2K210923833; Channel No.: 1


FREEZER TEMPERATURE RANGE : -15~-25°C

DATE : 31 Dec 2024 ~ 24 Jan 2025



2K210923833

— v1 2K210923833 [°C]  
Min Max Avg Sd MKT  
-22.1 -14.5 -19.68 0.59 -19.65

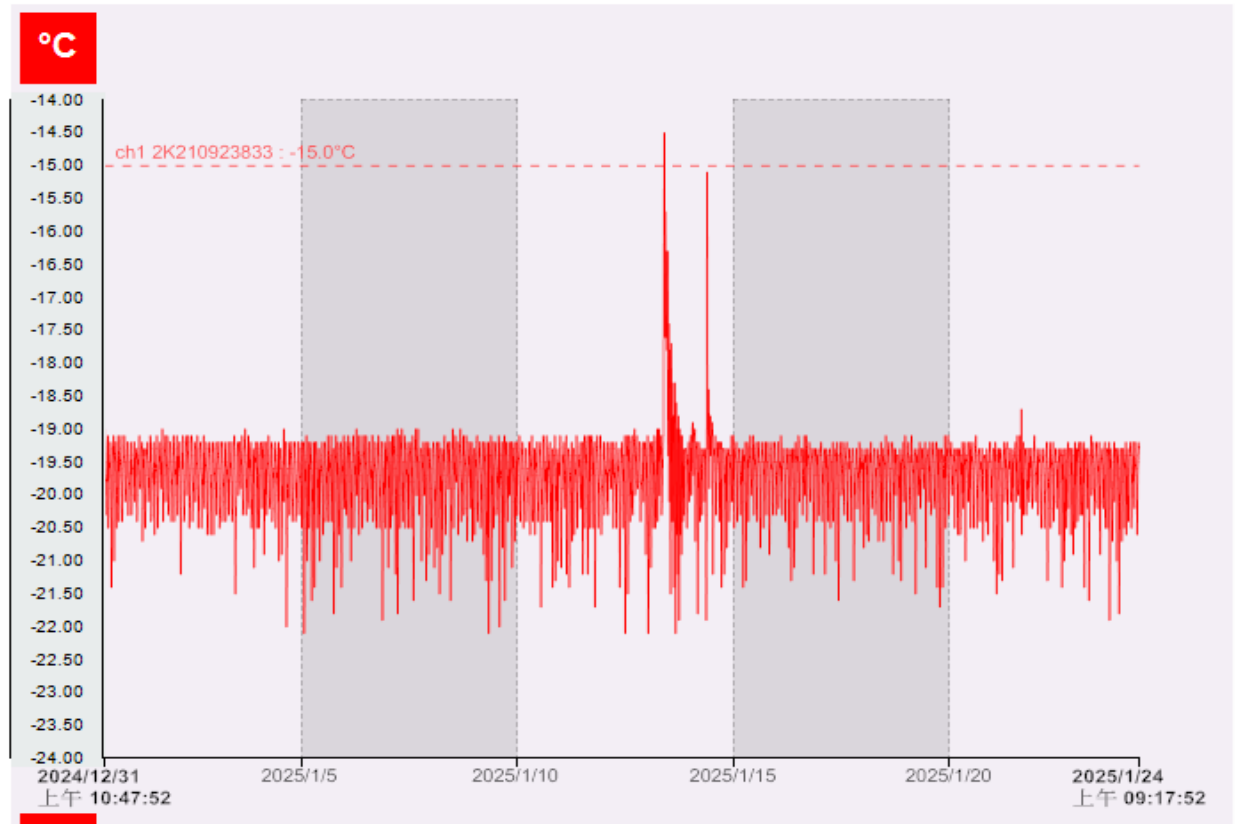

Comment:本冷凍櫃（冷凍2上層）目前無存放藥品。  
於2025年1月13日09:15 放入冰寶，暫時超溫。