

長庚紀念醫院—林口院區 藥品保存溫度記錄表


PHARMACY : B1 Medical Building , Clinical Research Pharmacy.

REFRIGERATOR : Manufacturer: PANASONIC; Model No.: MPR-1014R-PT; Serial No.: 15120037

THERMOMETER : Manufacturer: KIMO; Model No.: KTT-310; Serial No.: 1305 1583; Channel No.: 1

REFRIGERATOR TEMPERATURE RANGE : 2-8°C

DATE : 31 Dec 2024 ~ 24 Jan 2025

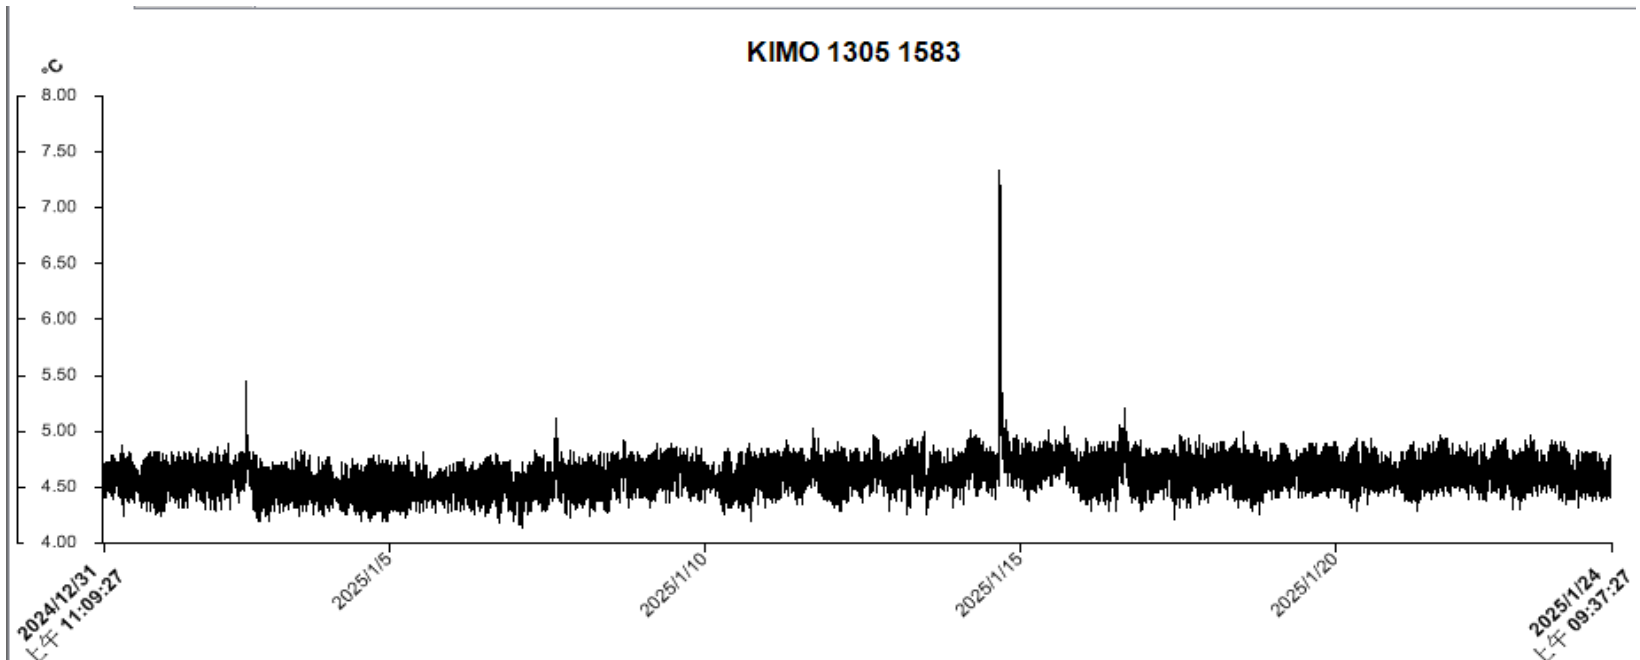

統計表

	#1
最小 T	4.14
最小 t	4.14
最大值 T	7.33
最大值 t	7.33
平均值 T	4.611
平均值 t	4.611
標準偏差 T	0.167
標準偏差 t	0.167
MKT T	4.611
MKT t	4.611

T: 整個週期
t: 顯示週期

Comment: